


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071318\
Data File : VV006596.D
Acq On : 13 Jul 2018 13:32
Operator : SY/MD
Sample : BFB65
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jul 14 00:30:59 2018

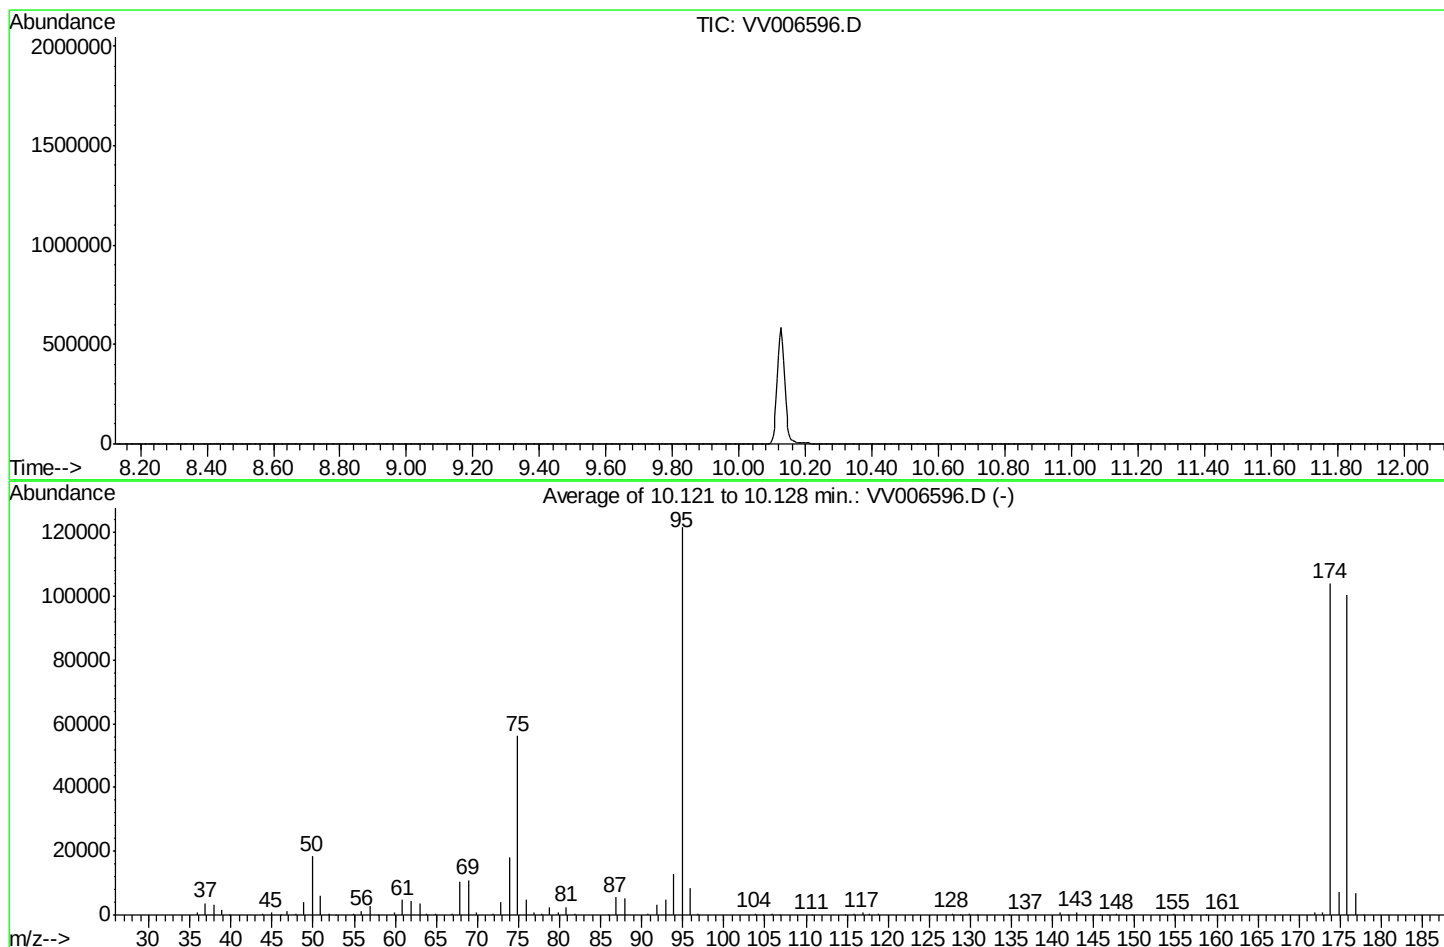

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	18464	PASS
75	95	30	80	46.2	56218	PASS
95	95	100	100	100.0	121685	PASS
96	95	5	9	6.9	8411	PASS
173	174	0.00	2	0.7	725	PASS
174	95	50	120	85.4	103882	PASS
175	174	5	9	7.0	7314	PASS
176	174	95	101	96.8	100517	PASS
177	176	5	9	6.7	6689	PASS

m/z	Abundance
39.80	136.0
43.80	708.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	618.0
36.90	3690.0
37.90	3226.0
38.90	1483.0
40.00	185.0
43.90	1051.0
44.90	839.0
46.00	126.0
46.90	1329.0
47.80	530.0
48.90	3740.0
49.90	17872.0
50.90	5791.0
51.90	222.0
54.90	263.0
55.90	1247.0
56.90	2547.0
59.90	925.0
60.90	4621.0
61.90	4481.0
63.00	3464.0
63.90	439.0
64.90	607.0
66.90	240.0
67.90	10463.0
68.90	10283.0
69.90	766.0
71.80	531.0
72.90	4052.0
73.90	17200.0
74.90	53744.0
76.00	4671.0
76.90	640.0
77.80	396.0
78.80	2283.0
79.90	820.0
80.90	2381.0
81.90	531.0
86.00	163.0
86.80	5386.0
87.90	4847.0
90.80	393.0
91.90	3136.0
92.90	4358.0
93.90	12214.0
94.90	115760.0
95.90	8090.0
96.90	235.0
103.80	470.0
104.70	194.0
105.90	365.0
106.80	123.0
110.70	102.0
114.70	110.0
115.80	345.0
116.90	677.0
117.70	291.0
118.80	469.0
127.80	378.0
128.80	145.0
129.80	358.0
130.70	147.0
134.70	182.0
136.80	157.0
140.90	792.0
142.90	921.0
144.90	178.0
145.70	162.0
147.80	233.0
149.60	141.0
154.80	293.0
156.90	184.0
158.70	118.0
160.70	150.0
171.80	708.0
172.90	647.0
173.80	95984.0
174.90	6836.0
175.80	92936.0
176.90	6393.0
177.80	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	713.0
36.90	3847.0
37.90	3301.0
38.90	1526.0
40.00	198.0
43.90	1094.0
44.90	807.0
46.00	121.0
46.90	1411.0
47.80	568.0
48.90	4031.0
49.90	19192.0
50.90	6200.0
51.90	246.0
54.90	247.0
55.90	1318.0
56.90	2756.0
57.90	111.0
59.90	1062.0
60.90	4839.0
61.90	4724.0
62.90	3682.0
63.80	468.0
64.90	565.0
66.90	241.0
67.90	10886.0
68.90	11338.0
69.90	847.0
71.80	554.0
72.90	4291.0
73.90	18816.0
74.90	58288.0
76.00	4992.0
76.90	679.0
77.80	457.0
78.80	2457.0
79.90	859.0
80.80	2581.0
81.90	597.0
86.00	187.0
86.80	5759.0
87.90	5347.0
90.80	410.0
91.90	3395.0
92.90	4814.0
93.90	13205.0
94.90	125904.0
95.90	8708.0
96.90	256.0
103.80	467.0
104.70	212.0
105.80	399.0
106.80	111.0
115.80	356.0
116.90	671.0
117.80	315.0
118.80	542.0
127.80	451.0
128.80	157.0
129.80	391.0
130.80	168.0
134.80	165.0
136.80	184.0
140.90	914.0
142.90	968.0
145.00	221.0
145.70	170.0
146.70	104.0
147.80	297.0
149.70	138.0
154.80	298.0
155.80	102.0
156.80	213.0
158.70	141.0
160.70	148.0
171.90	755.0
172.90	738.0
173.90	107328.0
174.90	7558.0
175.80	103912.0
176.90	6958.0
177.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	729.0
36.90	3729.0
37.90	3181.0
38.90	1418.0
39.90	188.0
43.90	1065.0
44.90	727.0
46.80	1377.0
47.90	588.0
48.90	3900.0
49.90	18328.0
50.90	5993.0
52.00	254.0
52.80	108.0
54.80	246.0
55.90	1305.0
56.90	2661.0
57.90	124.0
59.90	1022.0
60.90	4714.0
61.90	4557.0
62.90	3515.0
63.80	459.0
64.90	502.0
66.90	235.0
67.90	10303.0
68.90	11176.0
69.90	836.0
71.90	531.0
72.90	4235.0
73.90	18336.0
74.90	56624.0
76.00	4702.0
76.90	695.0
77.80	476.0
78.80	2392.0
79.90	813.0
80.80	2513.0
81.80	629.0
85.90	172.0
86.90	5633.0
87.90	5234.0
90.80	376.0
91.90	3257.0
92.90	4812.0
93.90	12987.0
94.90	123392.0
95.90	8437.0
96.90	242.0
103.80	415.0
104.70	195.0
105.80	389.0
106.90	104.0
115.80	340.0
116.90	582.0
117.80	342.0
118.80	585.0
127.70	458.0
128.80	168.0
129.80	414.0
130.80	173.0
134.80	147.0
136.80	190.0
140.90	901.0
141.80	103.0
142.90	980.0
144.90	230.0
145.70	155.0
147.80	330.0
149.70	101.0
154.70	335.0
155.80	108.0
156.80	238.0
158.70	146.0
160.70	133.0
171.90	749.0
172.80	792.0
173.90	108336.0
174.90	7548.0
175.80	104704.0
176.90	6718.0
177.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65