


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071320\
Data File : VV017456.D
Acq On : 13 Jul 2020 08:44
Operator : SY/MD
Sample : BFB61
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Title : VOC Analysis
Last Update : Tue Jul 14 05:08:48 2020

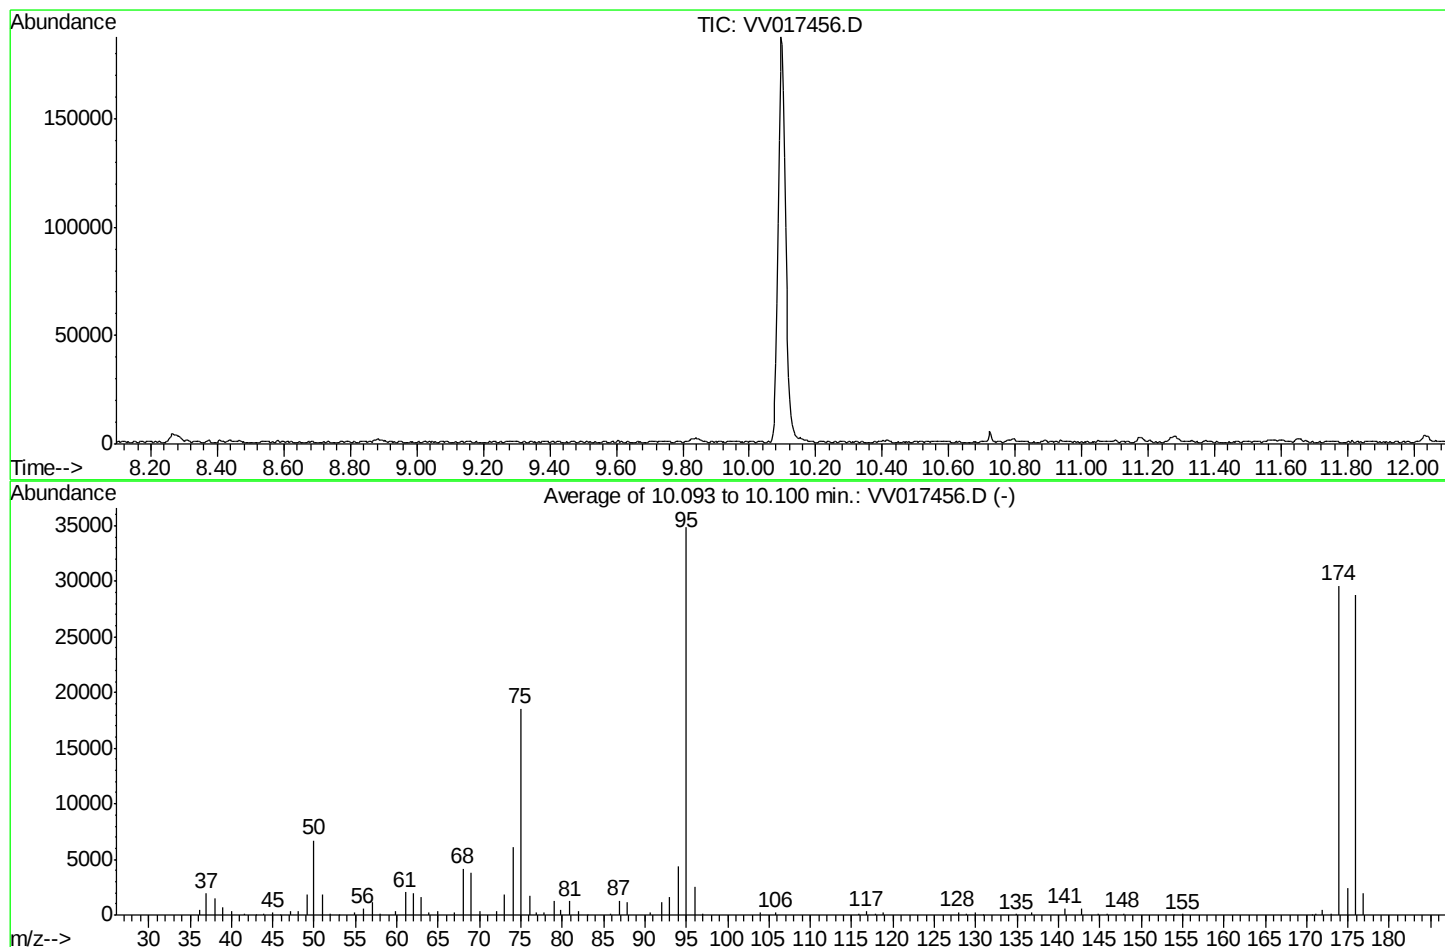

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	6689	PASS
75	95	30	80	53.3	18581	PASS
95	95	100	100	100.0	34856	PASS
96	95	5	9	7.2	2502	PASS
173	174	0.00	2	0.5	162	PASS
174	95	50	120	84.9	29597	PASS
175	174	5	9	8.2	2441	PASS
176	174	95	101	97.4	28832	PASS
177	176	5	9	6.7	1929	PASS

m/z	Abundance
36.10	449.0
37.00	1861.0
38.00	1426.0
39.00	663.0
40.00	314.0
41.60	116.0
44.00	358.0
45.00	271.0
47.20	330.0
48.00	256.0
49.10	1747.0
50.00	6653.0
51.10	1752.0
51.90	132.0
54.90	234.0
55.90	531.0
57.00	1140.0
59.80	362.0
61.00	1942.0
62.00	1857.0
63.00	1538.0
63.90	252.0
65.00	331.0
67.00	194.0
68.00	4008.0
69.00	3815.0
70.00	329.0
72.00	302.0
73.00	1872.0
74.00	5979.0
75.00	17752.0
76.10	1584.0
76.90	258.0
77.80	216.0
79.00	1298.0
79.80	420.0
80.90	1160.0
81.90	297.0
83.10	114.0
85.90	117.0
86.90	1189.0
87.90	987.0
90.70	254.0
92.00	1071.0
93.00	1596.0
94.10	4204.0
95.00	33040.0
96.00	2433.0
96.90	139.0
103.90	179.0
105.80	180.0
115.80	135.0
116.80	330.0
118.00	118.0
118.70	216.0
127.90	328.0
128.70	118.0
130.00	256.0
130.80	103.0
134.90	131.0
136.80	205.0
140.80	551.0
142.90	520.0
144.90	134.0
145.90	127.0
147.90	111.0
154.00	107.0
172.00	440.0
173.90	27592.0
175.00	2441.0
175.90	26600.0
176.90	1813.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.10	544.0
37.00	1951.0
38.00	1477.0
39.00	765.0
40.00	300.0
41.60	136.0
43.90	355.0
45.10	348.0
47.10	303.0
48.10	301.0
49.10	1911.0
50.00	6937.0
51.10	1831.0
51.90	131.0
53.10	109.0
54.90	282.0
56.00	580.0
57.00	1243.0
58.00	120.0
59.90	377.0
61.00	2129.0
62.00	2033.0
63.00	1642.0
63.90	244.0
65.00	353.0
67.00	213.0
68.00	4388.0
69.00	4020.0
70.00	416.0
72.00	314.0
73.00	1995.0
74.00	6273.0
75.00	19064.0
76.10	1759.0
76.90	252.0
77.80	214.0
79.00	1300.0
79.80	479.0
81.00	1288.0
82.00	341.0
85.90	132.0
86.90	1389.0
87.90	1215.0
90.70	227.0
92.00	1215.0
93.00	1643.0
94.00	4577.0
95.00	36392.0
96.00	2610.0
96.90	131.0
103.90	189.0
105.90	224.0
115.80	118.0
116.80	334.0
117.80	134.0
118.80	265.0
127.90	278.0
128.80	145.0
129.90	277.0
134.90	128.0
136.80	214.0
140.80	569.0
142.80	557.0
144.90	153.0
145.90	118.0
147.90	130.0
155.00	115.0
171.10	121.0
172.00	440.0
174.00	30584.0
175.00	2516.0
175.90	29872.0
176.90	2017.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.10	507.0
37.00	1902.0
38.00	1438.0
39.00	762.0
40.10	307.0
40.80	105.0
41.60	114.0
42.90	129.0
43.90	365.0
45.10	410.0
45.90	122.0
47.10	303.0
48.10	337.0
49.10	1746.0
50.00	6478.0
51.00	1790.0
51.90	102.0
55.00	244.0
56.00	574.0
57.00	1089.0
58.10	145.0
59.90	376.0
61.00	2038.0
62.10	1911.0
63.00	1542.0
63.90	225.0
64.90	398.0
67.00	222.0
68.00	4193.0
69.00	3696.0
70.00	404.0
72.00	297.0
73.00	1809.0
74.00	6050.0
75.00	18928.0
76.00	1796.0
76.90	233.0
77.70	171.0
79.00	1198.0
79.90	451.0
81.00	1289.0
81.90	365.0
85.80	129.0
86.90	1345.0
87.90	1200.0
90.70	180.0
92.00	1202.0
93.00	1566.0
94.00	4497.0
95.00	35464.0
96.00	2464.0
104.00	205.0
105.80	283.0
115.80	114.0
116.90	349.0
117.70	167.0
118.80	294.0
127.90	176.0
128.90	158.0
129.90	236.0
136.80	156.0
140.80	543.0
142.80	554.0
144.80	150.0
147.80	113.0
155.10	114.0
170.70	115.0
171.20	119.0
171.90	416.0
172.90	488.0
174.00	30616.0
175.00	2366.0
176.00	30024.0
176.90	1959.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
37.40	123.0
39.80	177.0
40.80	114.0
44.00	212.0
45.00	147.0
46.80	103.0
53.70	127.0
95.20	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61