

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021633.D
 Acq On : 13 Jul 2021 10:09
 Operator : SY/MD
 Sample : VV0713MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	257841	250391	14.37%	1.874%
2	1.561	155	162	179	rVB	182318	212091	12.17%	1.587%
3	2.104	321	331	346	rBV	384591	563180	32.31%	4.215%
4	2.625	491	493	494	rBV	327	133	0.01%	0.001%
5	2.706	516	518	523	rBV3	372	328	0.02%	0.002%
6	2.728	523	525	528	rBV4	414	276	0.02%	0.002%
7	2.805	545	549	552	rBV2	408	341	0.02%	0.003%
8	2.818	552	553	558	rVV2	192	161	0.01%	0.001%
9	2.879	569	572	573	rBV2	243	131	0.01%	0.001%
10	2.892	573	576	584	rVB4	628	625	0.04%	0.005%
11	2.947	587	593	598	rBV5	327	467	0.03%	0.003%
12	2.969	598	600	602	rBV	315	181	0.01%	0.001%
13	3.059	624	628	630	rBV2	264	206	0.01%	0.002%
14	3.095	636	639	642	rBV2	692	388	0.02%	0.003%
15	3.108	642	643	648	rVB	252	132	0.01%	0.001%
16	3.133	648	651	652	rBV2	329	172	0.01%	0.001%
17	3.172	660	663	665	rBV2	216	144	0.01%	0.001%
18	3.182	665	666	671	rVB	411	215	0.01%	0.002%
19	3.220	671	678	679	rBV2	324	316	0.02%	0.002%
20	3.355	716	720	725	rBV2	339	290	0.02%	0.002%
21	3.397	732	733	736	rVB	465	182	0.01%	0.001%
22	3.458	750	752	756	rVB2	236	150	0.01%	0.001%
23	3.477	756	758	763	rBV3	320	152	0.01%	0.001%
24	3.516	768	770	774	rVB2	442	353	0.02%	0.003%
25	3.542	774	778	779	rBV	348	230	0.01%	0.002%
26	3.635	802	807	809	rBV2	289	267	0.02%	0.002%
27	3.674	814	819	820	rBV	331	222	0.01%	0.002%
28	3.712	829	831	835	rBV2	397	234	0.01%	0.002%
29	3.741	838	840	843	rVB3	277	165	0.01%	0.001%
30	3.764	843	847	851	rBV3	357	375	0.02%	0.003%
31	3.866	869	879	918	rBV	147321	385183	22.10%	2.883%
32	4.346	1013	1028	1058	rBV	268146	666743	38.26%	4.991%
33	4.677	1129	1131	1132	rBV	391	142	0.01%	0.001%
34	4.799	1166	1169	1172	rVB3	485	292	0.02%	0.002%
35	4.821	1173	1176	1178	rBV2	382	211	0.01%	0.002%
36	4.860	1184	1188	1190	rBV	423	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021633.D
 Acq On : 13 Jul 2021 10:09
 Operator : SY/MD
 Sample : VV0713MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	4.905	1201	1202	1206	rVB3	345	154	0.01%	0.001%
38	5.043	1223	1245	1282	rBV2	680916	1742804	100.00%	13.045%
39	5.532	1394	1397	1398	rBV	672	348	0.02%	0.003%
40	5.612	1409	1422	1448	rBV	519007	1056842	60.64%	7.910%
41	5.908	1502	1514	1528	rBV3	14755	32578	1.87%	0.244%
42	6.069	1550	1564	1599	rBV	380387	783840	44.98%	5.867%
43	6.365	1652	1656	1660	rVB2	560	506	0.03%	0.004%
44	6.390	1660	1664	1667	rBV2	412	326	0.02%	0.002%
45	6.407	1667	1669	1674	rVB2	579	291	0.02%	0.002%
46	6.426	1674	1675	1681	rVB2	272	153	0.01%	0.001%
47	6.500	1695	1698	1700	rBV2	356	262	0.02%	0.002%
48	6.538	1708	1710	1714	rBV2	297	180	0.01%	0.001%
49	6.606	1730	1731	1734	rBV	213	145	0.01%	0.001%
50	6.641	1736	1742	1744	rBV5	645	749	0.04%	0.006%
51	6.690	1755	1757	1762	rVB3	730	403	0.02%	0.003%
52	6.728	1766	1769	1772	rVB4	375	214	0.01%	0.002%
53	6.786	1783	1787	1791	rVB2	353	251	0.01%	0.002%
54	6.808	1791	1794	1797	rVB3	357	223	0.01%	0.002%
55	6.850	1801	1807	1808	rBV2	297	196	0.01%	0.001%
56	6.985	1835	1849	1874	rBV	235205	426460	24.47%	3.192%
57	7.313	1939	1951	1970	rBV	835824	1455528	83.52%	10.895%
58	7.558	2025	2027	2031	rVB3	515	308	0.02%	0.002%
59	7.622	2036	2047	2080	rVV	157170	278704	15.99%	2.086%
60	7.876	2124	2126	2128	rBV	347	197	0.01%	0.001%
61	7.908	2132	2136	2139	rBV3	301	252	0.01%	0.002%
62	8.008	2164	2167	2170	rBV2	312	147	0.01%	0.001%
63	8.085	2181	2191	2234	rBV	454183	849547	48.75%	6.359%
64	8.452	2303	2305	2307	rBV	354	182	0.01%	0.001%
65	8.525	2321	2328	2331	rBV2	447	623	0.04%	0.005%
66	8.561	2335	2339	2342	rBV4	401	333	0.02%	0.002%
67	8.609	2352	2354	2355	rBV4	348	155	0.01%	0.001%
68	8.680	2374	2376	2380	rVB2	308	184	0.01%	0.001%
69	8.728	2390	2391	2397	rVB	564	208	0.01%	0.002%
70	8.754	2397	2399	2404	rBV	422	342	0.02%	0.003%
71	8.853	2418	2430	2460	rBV	769416	1266541	72.67%	9.480%
72	9.204	2537	2539	2542	rVB2	368	153	0.01%	0.001%
73	9.259	2554	2556	2559	rVB	318	139	0.01%	0.001%
74	9.320	2572	2575	2580	rVB3	590	340	0.02%	0.003%
75	9.397	2597	2599	2602	rVV2	362	275	0.02%	0.002%
76	9.410	2602	2603	2610	rVB2	499	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021633.D
 Acq On : 13 Jul 2021 10:09
 Operator : SY/MD
 Sample : VV0713MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.538	2640	2643	2644	rBV2	511	291	0.02%	0.002%
78	9.673	2680	2685	2688	rBV3	782	699	0.04%	0.005%
79	9.750	2706	2709	2712	rVB	712	386	0.02%	0.003%
80	9.812	2723	2728	2731	rBV2	320	276	0.02%	0.002%
81	9.937	2763	2767	2769	rBV5	781	621	0.04%	0.005%
82	9.979	2778	2780	2784	rBV3	268	199	0.01%	0.001%
83	10.021	2789	2793	2795	rBV3	505	327	0.02%	0.002%
84	10.127	2818	2826	2835	rVB3	5872	9065	0.52%	0.068%
85	10.217	2842	2854	2877	rBV	522843	821445	47.13%	6.148%
86	10.538	2951	2954	2955	rBV	709	357	0.02%	0.003%
87	10.660	2984	2992	2993	rBV4	1115	1161	0.07%	0.009%
88	10.725	3009	3012	3014	rBV2	365	203	0.01%	0.002%
89	10.738	3014	3016	3017	rBV	405	197	0.01%	0.001%
90	10.918	3063	3072	3081	rBV4	7227	10285	0.59%	0.077%
91	11.094	3124	3127	3130	rVB	402	277	0.02%	0.002%
92	11.146	3137	3143	3152	rBV7	2876	3968	0.23%	0.030%
93	11.249	3164	3175	3198	rBV	796276	1239081	71.10%	9.274%
94	11.625	3280	3292	3312	rBV	817835	1263022	72.47%	9.454%
95	11.934	3386	3388	3391	rBV3	488	254	0.01%	0.002%
96	12.657	3606	3613	3620	rVB3	2119	3028	0.17%	0.023%
97	12.747	3639	3641	3644	rBV	464	230	0.01%	0.002%
98	13.268	3796	3803	3811	rBV5	3003	4696	0.27%	0.035%
99	13.516	3874	3880	3894	rVB2	4615	7553	0.43%	0.057%
100	13.750	3946	3953	3961	rVB7	3578	5885	0.34%	0.044%




Sum of corrected areas: 13360167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021633.D
Acq On : 13 Jul 2021 10:09
Operator : SY/MD
Sample : VV0713MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

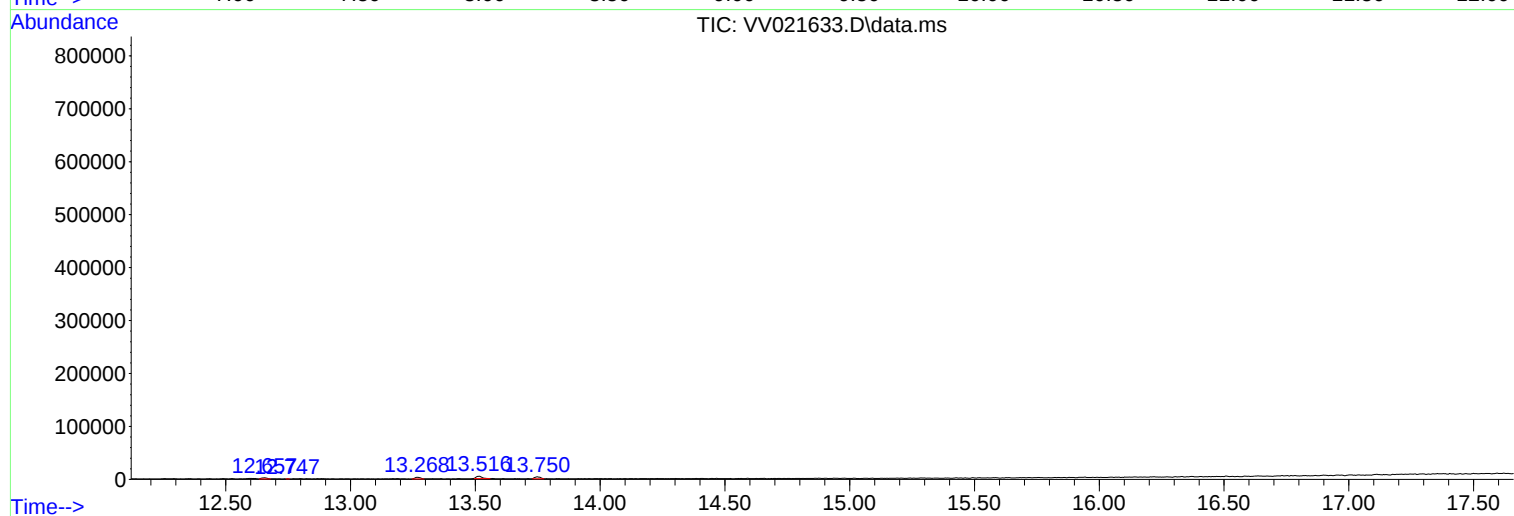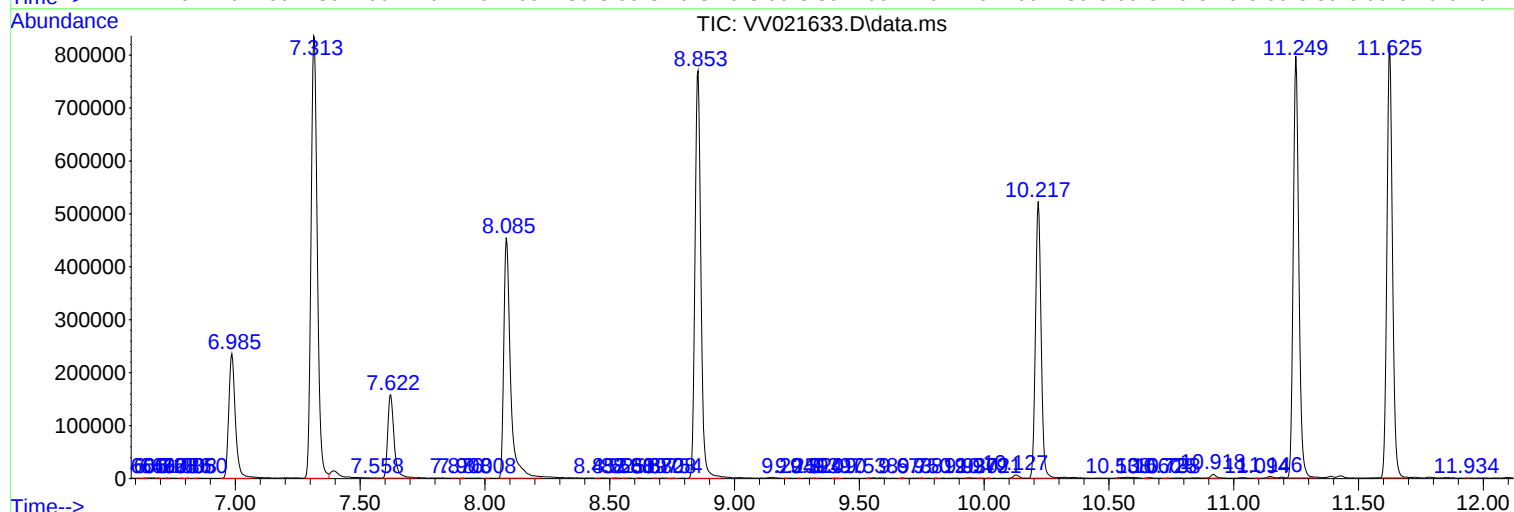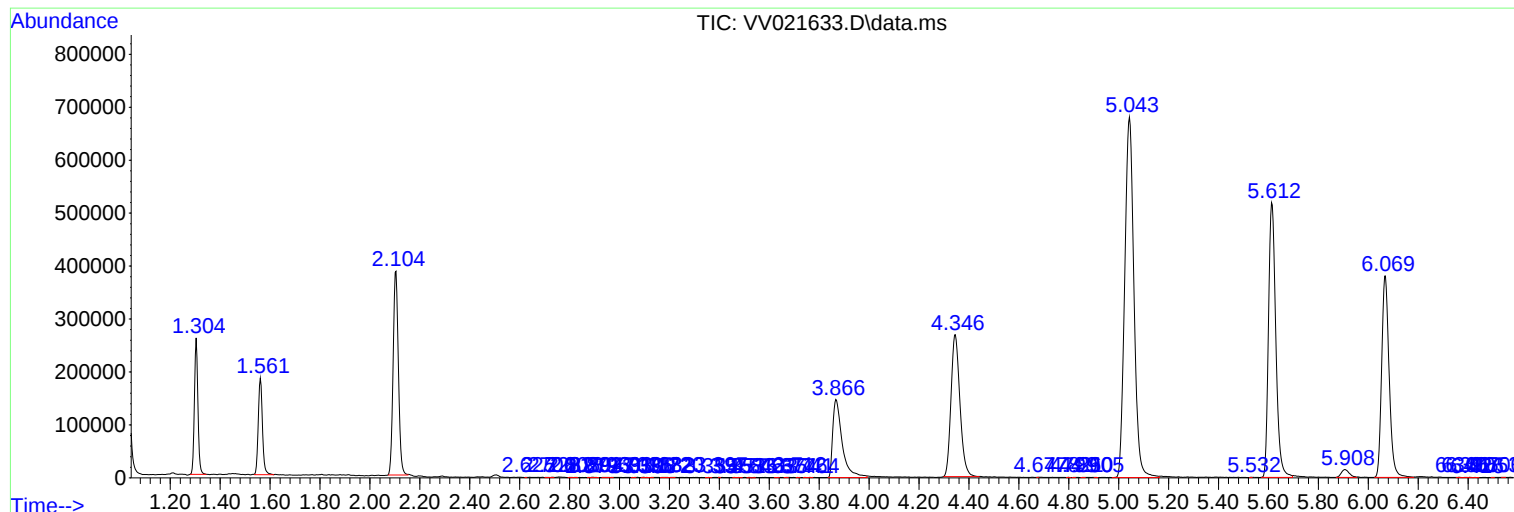

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021633.D
Acq On : 13 Jul 2021 10:09
Operator : SY/MD
Sample : VV0713MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021633.D
Acq On : 13 Jul 2021 10:09
Operator : SY/MD
Sample : VV0713MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
