

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021634.D
 Acq On : 13 Jul 2021 10:33
 Operator : SY/MD
 Sample : VV0713WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

Signal : TIC: VV021634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	241802	236961	14.03%	1.828%
2	1.558	154	161	177	rVB	172255	198889	11.78%	1.534%
3	2.105	321	331	348	rBV	365812	537053	31.80%	4.142%
4	2.709	517	519	522	rBV	309	149	0.01%	0.001%
5	2.777	539	540	542	rVB2	518	159	0.01%	0.001%
6	2.831	555	557	559	rBV2	374	215	0.01%	0.002%
7	2.876	568	571	572	rBV	270	163	0.01%	0.001%
8	3.050	621	625	631	rVB5	551	468	0.03%	0.004%
9	3.159	655	659	661	rBV3	407	378	0.02%	0.003%
10	3.195	667	670	672	rBV2	235	140	0.01%	0.001%
11	3.214	674	676	678	rBV	259	141	0.01%	0.001%
12	3.307	701	705	709	rVB3	464	301	0.02%	0.002%
13	3.365	717	723	726	rBV2	302	279	0.02%	0.002%
14	3.439	742	746	748	rBV	353	309	0.02%	0.002%
15	3.503	763	766	768	rBV	372	190	0.01%	0.001%
16	3.609	796	799	801	rBV2	225	110	0.01%	0.001%
17	3.629	802	805	810	rVV2	458	281	0.02%	0.002%
18	3.667	815	817	820	rBV	309	199	0.01%	0.002%
19	3.712	828	831	834	rBV2	220	170	0.01%	0.001%
20	3.744	839	841	845	rVB2	442	235	0.01%	0.002%
21	3.870	870	880	915	rBV	149477	389281	23.05%	3.002%
22	4.349	1014	1029	1058	rVB	261050	645521	38.22%	4.979%
23	4.683	1130	1133	1134	rBV2	581	285	0.02%	0.002%
24	4.735	1146	1149	1150	rBV	432	227	0.01%	0.002%
25	4.831	1176	1179	1181	rBV	323	222	0.01%	0.002%
26	4.915	1202	1205	1208	rBV2	317	170	0.01%	0.001%
27	5.047	1228	1246	1277	rBV2	659766	1688998	100.00%	13.026%
28	5.320	1326	1331	1333	rBV3	789	762	0.05%	0.006%
29	5.503	1386	1388	1389	rBV	371	196	0.01%	0.002%
30	5.574	1407	1410	1411	rBV	420	212	0.01%	0.002%
31	5.616	1411	1423	1453	rVV	503158	1013885	60.03%	7.819%
32	5.908	1503	1514	1531	rBV3	12718	28262	1.67%	0.218%
33	6.069	1549	1564	1593	rBV	366761	754758	44.69%	5.821%
34	6.291	1631	1633	1637	rVB3	502	360	0.02%	0.003%
35	6.358	1652	1654	1655	rBV3	264	130	0.01%	0.001%
36	6.400	1666	1667	1670	rVB3	396	167	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021634.D
 Acq On : 13 Jul 2021 10:33
 Operator : SY/MD
 Sample : VV0713WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.420	1670	1673	1675	rBV	444	276	0.02%	0.002%
38	6.436	1675	1678	1681	rVB2	251	155	0.01%	0.001%
39	6.465	1682	1687	1691	rVB3	597	451	0.03%	0.003%
40	6.526	1700	1706	1710	rBV3	490	569	0.03%	0.004%
41	6.548	1711	1713	1715	rBV2	329	143	0.01%	0.001%
42	6.638	1735	1741	1742	rBV2	643	460	0.03%	0.004%
43	6.738	1770	1772	1776	rBV3	464	336	0.02%	0.003%
44	6.812	1790	1795	1797	rVV	175	151	0.01%	0.001%
45	6.828	1797	1800	1803	rVB2	353	221	0.01%	0.002%
46	6.847	1803	1806	1808	rBV2	429	269	0.02%	0.002%
47	6.876	1812	1815	1817	rBV2	227	139	0.01%	0.001%
48	6.937	1833	1834	1837	rBV	425	189	0.01%	0.001%
49	6.989	1838	1850	1875	rBV	223636	409243	24.23%	3.156%
50	7.317	1940	1952	1970	rBV	807556	1400955	82.95%	10.805%
51	7.516	2012	2014	2019	rVB3	914	447	0.03%	0.003%
52	7.622	2037	2047	2073	rBV	155169	271252	16.06%	2.092%
53	7.834	2111	2113	2115	rBV2	256	116	0.01%	0.001%
54	7.905	2132	2135	2138	rVB4	423	327	0.02%	0.003%
55	7.921	2138	2140	2143	rBV2	436	309	0.02%	0.002%
56	7.982	2155	2159	2160	rBV2	535	375	0.02%	0.003%
57	8.021	2170	2171	2174	rBV	451	243	0.01%	0.002%
58	8.088	2182	2192	2246	rBV	467682	867070	51.34%	6.687%
59	8.391	2284	2286	2289	rBV3	473	350	0.02%	0.003%
60	8.580	2342	2345	2347	rVB2	391	234	0.01%	0.002%
61	8.603	2347	2352	2356	rBV4	747	633	0.04%	0.005%
62	8.628	2356	2360	2363	rBV3	470	426	0.03%	0.003%
63	8.667	2370	2372	2375	rVB	423	225	0.01%	0.002%
64	8.686	2375	2378	2379	rBV	401	174	0.01%	0.001%
65	8.751	2396	2398	2400	rVV	450	266	0.02%	0.002%
66	8.792	2407	2411	2413	rBV2	367	231	0.01%	0.002%
67	8.854	2418	2430	2468	rBV	758579	1221910	72.35%	9.424%
68	9.095	2503	2505	2508	rVB	478	211	0.01%	0.002%
69	9.149	2518	2522	2528	rBV4	1862	1905	0.11%	0.015%
70	9.378	2591	2593	2594	rBV4	406	146	0.01%	0.001%
71	9.413	2602	2604	2605	rBV	314	130	0.01%	0.001%
72	9.474	2620	2623	2628	rVB2	446	281	0.02%	0.002%
73	9.503	2630	2632	2635	rBV2	245	140	0.01%	0.001%
74	9.538	2642	2643	2646	rBV	341	151	0.01%	0.001%
75	9.638	2672	2674	2680	rVB3	737	509	0.03%	0.004%
76	9.683	2684	2688	2693	rVB3	550	541	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021634.D
 Acq On : 13 Jul 2021 10:33
 Operator : SY/MD
 Sample : VV0713WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK214

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.796	2718	2723	2727	rBV	336	372	0.02%	0.003%
78	9.831	2731	2734	2735	rBV	270	127	0.01%	0.001%
79	9.934	2764	2766	2767	rBV	566	240	0.01%	0.002%
80	9.982	2778	2781	2786	rVB3	445	269	0.02%	0.002%
81	10.011	2786	2790	2794	rBV3	395	354	0.02%	0.003%
82	10.130	2818	2827	2842	rVB2	5303	8750	0.52%	0.067%
83	10.217	2842	2854	2875	rBV	517041	820736	48.59%	6.330%
84	10.423	2914	2918	2919	rBV	189	111	0.01%	0.001%
85	10.542	2952	2955	2956	rBV	618	338	0.02%	0.003%
86	10.651	2987	2989	2991	rBV2	554	338	0.02%	0.003%
87	10.770	3023	3026	3031	rBV3	690	692	0.04%	0.005%
88	10.918	3063	3072	3082	rVB4	6012	9458	0.56%	0.073%
89	10.960	3082	3085	3088	rBV2	449	324	0.02%	0.002%
90	10.995	3093	3096	3098	rVV2	427	232	0.01%	0.002%
91	11.037	3102	3109	3117	rVB5	1190	2049	0.12%	0.016%
92	11.072	3118	3120	3123	rBV	335	122	0.01%	0.001%
93	11.146	3137	3143	3145	rBV4	2466	2818	0.17%	0.022%
94	11.249	3164	3175	3197	rBV	755719	1197531	70.90%	9.236%
95	11.625	3280	3292	3311	rBV	783412	1235251	73.14%	9.527%
96	11.776	3335	3339	3340	rBV4	1212	882	0.05%	0.007%
97	11.988	3403	3405	3409	rBV3	432	318	0.02%	0.002%
98	12.249	3480	3486	3489	rBV4	840	920	0.05%	0.007%
99	12.535	3574	3575	3579	rBV2	426	250	0.01%	0.002%
100	12.593	3587	3593	3597	rBV5	866	1264	0.07%	0.010%




Sum of corrected areas: 12966131

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021634.D
Acq On : 13 Jul 2021 10:33
Operator : SY/MD
Sample : VV0713WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

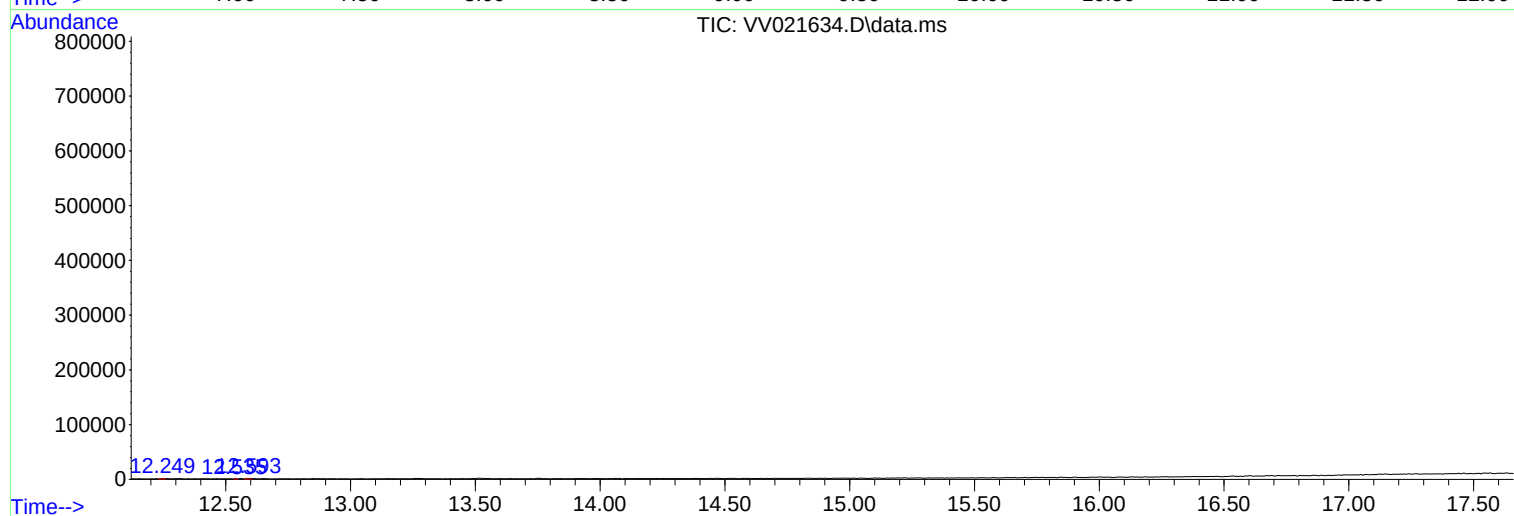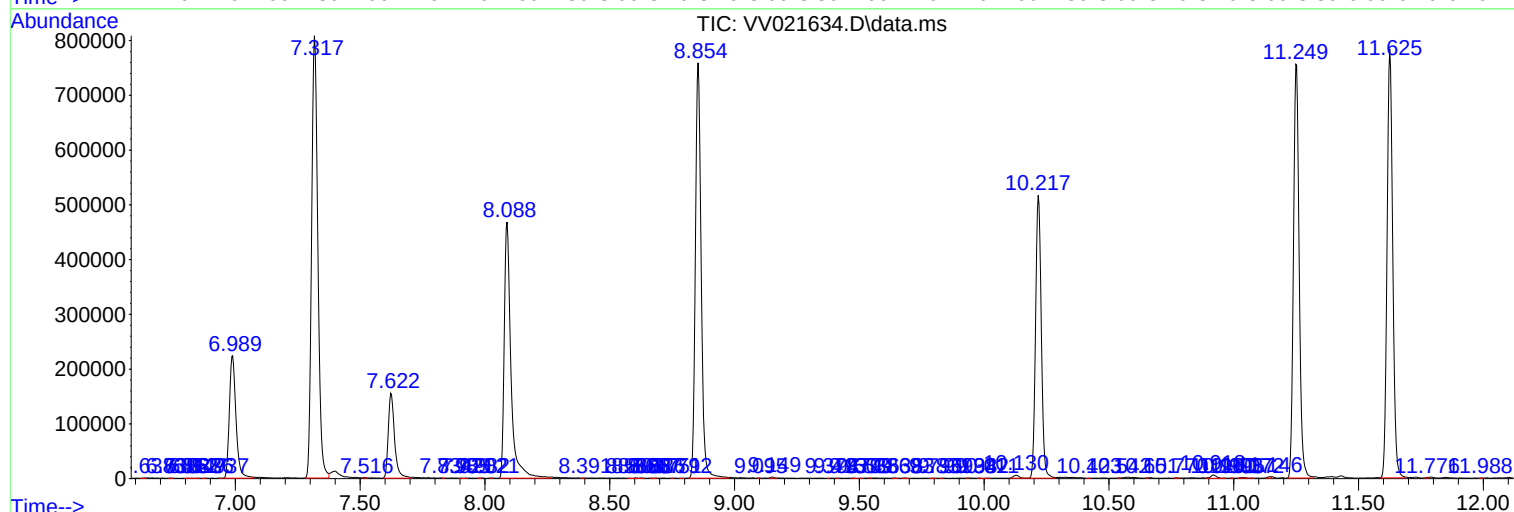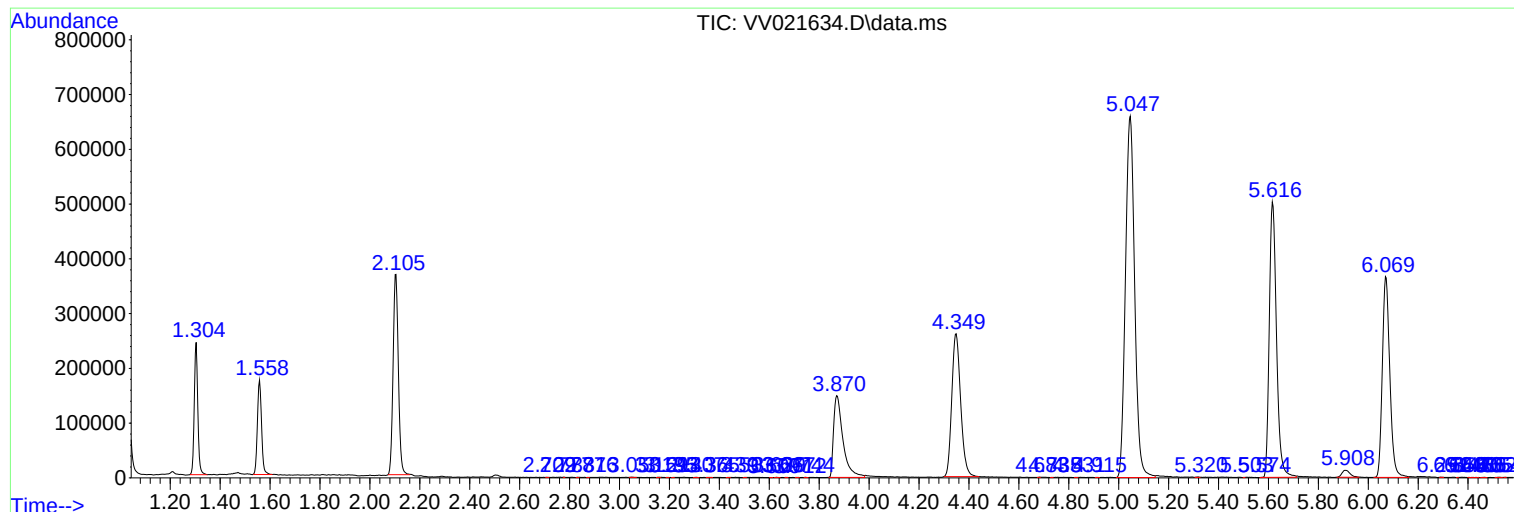

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021634.D
Acq On : 13 Jul 2021 10:33
Operator : SY/MD
Sample : VV0713WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021634.D
Acq On : 13 Jul 2021 10:33
Operator : SY/MD
Sample : VV0713WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
