

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021635.D
 Acq On : 13 Jul 2021 10:57
 Operator : SY/MD
 Sample : M2970-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rBV	231755	226807	13.78%	1.786%
2	1.558	154	161	172	rBV	163639	190529	11.58%	1.501%
3	2.105	321	331	356	rVB	352176	518835	31.52%	4.086%
4	2.449	436	438	442	rBV3	746	428	0.03%	0.003%
5	2.664	503	505	508	rBV	370	218	0.01%	0.002%
6	2.748	527	531	533	rBV2	655	426	0.03%	0.003%
7	2.870	564	569	572	rBV2	482	462	0.03%	0.004%
8	2.886	572	574	576	rBV	396	147	0.01%	0.001%
9	2.934	587	589	590	rBV	248	118	0.01%	0.001%
10	3.143	650	654	656	rBV2	368	241	0.01%	0.002%
11	3.333	709	713	715	rBV2	471	302	0.02%	0.002%
12	3.384	727	729	731	rBV2	134	76	0.00%	0.001%
13	3.404	734	735	739	rVB	320	195	0.01%	0.002%
14	3.465	751	754	758	rBV2	364	186	0.01%	0.001%
15	3.484	758	760	762	rVB	262	131	0.01%	0.001%
16	3.513	765	769	772	rBV2	380	380	0.02%	0.003%
17	3.555	777	782	784	rBV3	350	311	0.02%	0.002%
18	3.603	794	797	798	rVV	170	97	0.01%	0.001%
19	3.632	804	806	811	rVB2	259	174	0.01%	0.001%
20	3.680	819	821	822	rBV	291	100	0.01%	0.001%
21	3.716	829	832	836	rVB3	454	293	0.02%	0.002%
22	3.735	836	838	841	rBV	126	83	0.01%	0.001%
23	3.757	842	845	849	rVB	396	193	0.01%	0.002%
24	3.777	849	851	854	rBV	195	101	0.01%	0.001%
25	3.873	871	881	915	rBV	156093	401870	24.42%	3.165%
26	4.349	1013	1029	1056	rBV2	256353	630371	38.30%	4.965%
27	4.661	1124	1126	1127	rBV2	395	179	0.01%	0.001%
28	4.754	1152	1155	1157	rBV	480	289	0.02%	0.002%
29	4.783	1163	1164	1166	rBV	274	95	0.01%	0.001%
30	4.822	1171	1176	1180	rBV3	532	661	0.04%	0.005%
31	4.851	1183	1185	1189	rVB	267	175	0.01%	0.001%
32	4.870	1189	1191	1194	rBV2	260	93	0.01%	0.001%
33	4.892	1196	1198	1199	rBV2	178	72	0.00%	0.001%
34	4.970	1219	1222	1226	rVB4	412	235	0.01%	0.002%
35	5.047	1226	1246	1272	rBV2	642589	1645911	100.00%	12.963%
36	5.503	1386	1388	1390	rBV	385	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071321\
 Data File : VW021635.D
 Acq On : 13 Jul 2021 10:57
 Operator : SY/MD
 Sample : M2970-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.552	1401	1403	1405	rVB2	583	251	0.02%	0.002%
38	5.574	1408	1410	1411	rBV	244	133	0.01%	0.001%
39	5.619	1411	1424	1449	rBV	488039	980878	59.59%	7.725%
40	5.908	1504	1514	1539	rVB3	14772	32377	1.97%	0.255%
41	6.005	1542	1544	1547	rBV2	352	227	0.01%	0.002%
42	6.072	1550	1565	1594	rBV	361021	745962	45.32%	5.875%
43	6.298	1633	1635	1636	rVB2	578	157	0.01%	0.001%
44	6.343	1648	1649	1650	rBV	328	65	0.00%	0.001%
45	6.359	1650	1654	1656	rBV2	371	245	0.01%	0.002%
46	6.384	1660	1662	1663	rBV2	302	126	0.01%	0.001%
47	6.436	1674	1678	1682	rBV3	420	450	0.03%	0.004%
48	6.481	1689	1692	1693	rBV	160	83	0.01%	0.001%
49	6.587	1722	1725	1732	rBV3	429	401	0.02%	0.003%
50	6.619	1732	1735	1737	rVB	493	252	0.02%	0.002%
51	6.642	1737	1742	1745	rBV3	962	1003	0.06%	0.008%
52	6.764	1778	1780	1782	rBV	240	109	0.01%	0.001%
53	6.786	1785	1787	1790	rVB2	197	94	0.01%	0.001%
54	6.825	1797	1799	1803	rBV	388	155	0.01%	0.001%
55	6.847	1803	1806	1809	rBV3	222	132	0.01%	0.001%
56	6.863	1809	1811	1813	rBV	184	80	0.00%	0.001%
57	6.883	1814	1817	1818	rBV	214	114	0.01%	0.001%
58	6.921	1822	1829	1835	rBV4	345	577	0.04%	0.005%
59	6.989	1838	1850	1879	rBV	223598	408056	24.79%	3.214%
60	7.224	1922	1923	1928	rVB5	885	498	0.03%	0.004%
61	7.317	1940	1952	1971	rBV	785954	1354323	82.28%	10.666%
62	7.622	2037	2047	2068	rBV	153902	264330	16.06%	2.082%
63	7.896	2130	2132	2135	rVB	440	202	0.01%	0.002%
64	7.986	2156	2160	2165	rBV4	654	428	0.03%	0.003%
65	8.088	2179	2192	2230	rBV	487898	890918	54.13%	7.017%
66	8.503	2319	2321	2324	rBV2	500	261	0.02%	0.002%
67	8.587	2346	2347	2349	rBV	244	117	0.01%	0.001%
68	8.735	2391	2393	2395	rBV	184	68	0.00%	0.001%
69	8.767	2401	2403	2405	rBV	324	113	0.01%	0.001%
70	8.854	2418	2430	2454	rBV	722762	1185085	72.00%	9.333%
71	9.095	2501	2505	2508	rBV3	540	487	0.03%	0.004%
72	9.378	2590	2593	2594	rBV	284	138	0.01%	0.001%
73	9.391	2594	2597	2599	rVV2	194	126	0.01%	0.001%
74	9.471	2621	2622	2624	rBV	224	103	0.01%	0.001%
75	9.683	2683	2688	2693	rVB3	631	591	0.04%	0.005%
76	9.731	2701	2703	2705	rVB	345	134	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021635.D
 Acq On : 13 Jul 2021 10:57
 Operator : SY/MD
 Sample : M2970-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.796	2719	2723	2726	rBV2	282	223	0.01%	0.002%
78	9.818	2726	2730	2734	rVB2	348	214	0.01%	0.002%
79	9.879	2747	2749	2753	rBV3	267	167	0.01%	0.001%
80	9.947	2768	2770	2774	rVB2	405	228	0.01%	0.002%
81	10.005	2786	2788	2791	rBV	221	145	0.01%	0.001%
82	10.024	2791	2794	2796	rVV2	417	245	0.01%	0.002%
83	10.082	2808	2812	2814	rBV2	402	281	0.02%	0.002%
84	10.127	2817	2826	2837	rVV2	5177	8669	0.53%	0.068%
85	10.217	2842	2854	2877	rBV	520941	828099	50.31%	6.522%
86	10.423	2917	2918	2921	rBV	355	178	0.01%	0.001%
87	10.442	2923	2924	2925	rBV	460	152	0.01%	0.001%
88	10.657	2987	2991	2993	rBV2	565	588	0.04%	0.005%
89	10.735	3013	3015	3017	rBV2	201	96	0.01%	0.001%
90	10.783	3027	3030	3031	rBV2	321	167	0.01%	0.001%
91	10.976	3085	3090	3095	rBV4	627	555	0.03%	0.004%
92	11.098	3126	3128	3129	rBV4	283	106	0.01%	0.001%
93	11.146	3136	3143	3153	rVB6	2923	4356	0.26%	0.034%
94	11.204	3159	3161	3163	rBV3	643	272	0.02%	0.002%
95	11.249	3164	3175	3206	rBV	732257	1160295	70.50%	9.138%
96	11.625	3281	3292	3314	rBV	762091	1200619	72.95%	9.456%
97	11.837	3356	3358	3359	rBV	679	306	0.02%	0.002%
98	11.989	3402	3405	3409	rBV2	445	355	0.02%	0.003%
99	12.320	3505	3508	3511	rVB	290	162	0.01%	0.001%
100	12.715	3629	3631	3633	rBV	278	131	0.01%	0.001%




Sum of corrected areas: 12697468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021635.D
Acq On : 13 Jul 2021 10:57
Operator : SY/MD
Sample : M2970-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

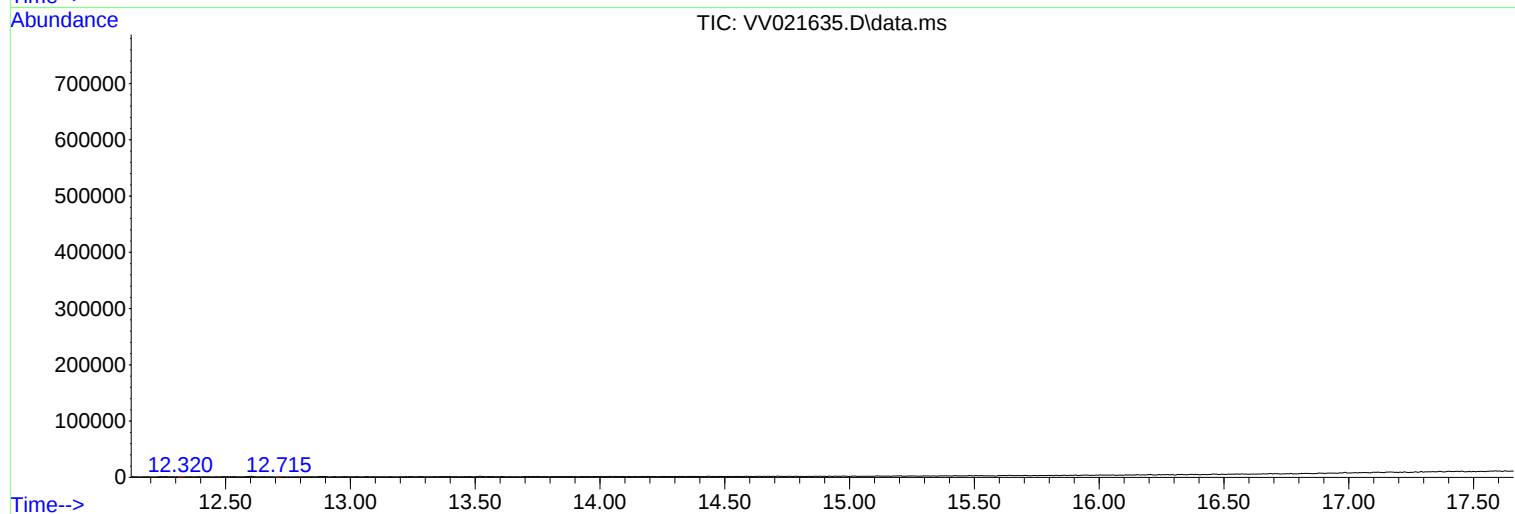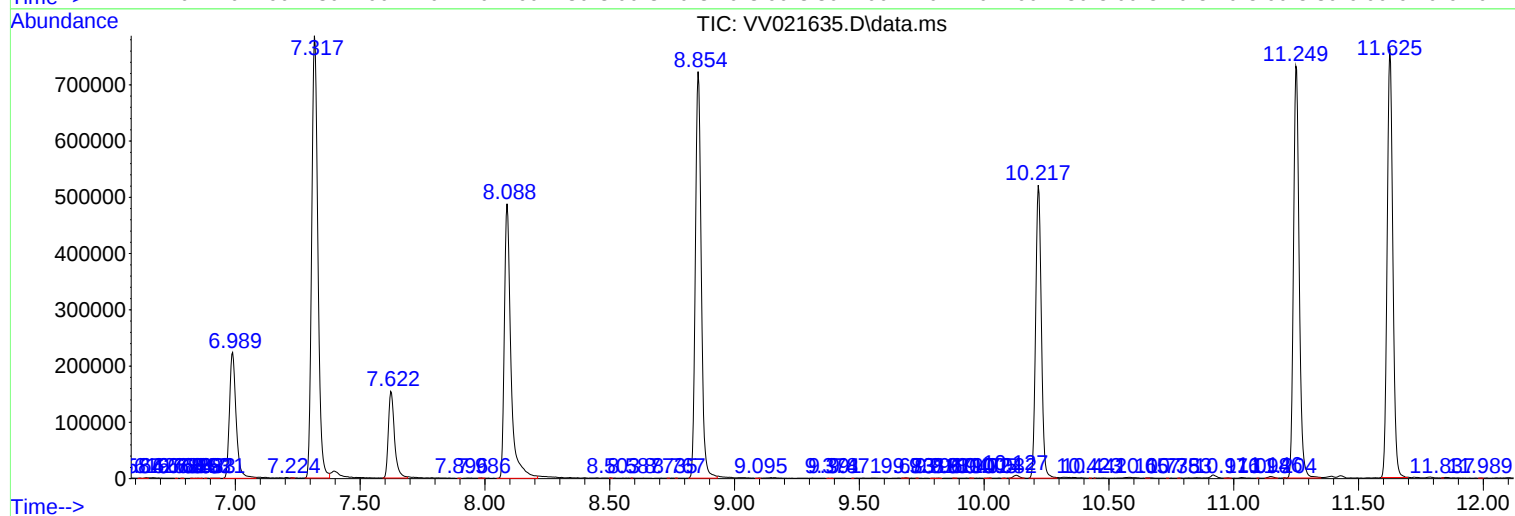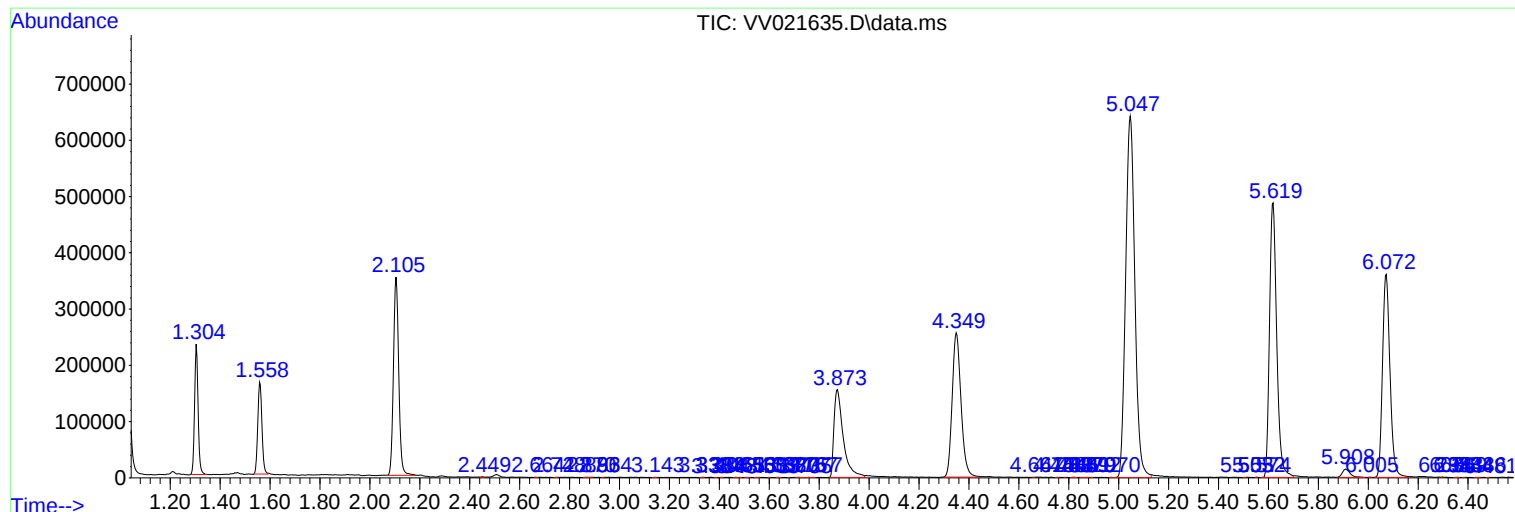

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021635.D
Acq On : 13 Jul 2021 10:57
Operator : SY/MD
Sample : M2970-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021635.D
Acq On : 13 Jul 2021 10:57
Operator : SY/MD
Sample : M2970-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
