

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021637.D
 Acq On : 13 Jul 2021 11:45
 Operator : SY/MD
 Sample : M3008-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	248297	244779	14.00%	1.763%
2	1.558	154	161	176	rVB	184019	211021	12.07%	1.519%
3	2.105	322	331	343	rBV	380691	555063	31.74%	3.997%
4	2.622	483	492	495	rBV5	2383	3853	0.22%	0.028%
5	2.722	521	523	526	rBV3	499	354	0.02%	0.003%
6	2.786	541	543	545	rBV2	367	202	0.01%	0.001%
7	2.860	563	566	568	rBV2	362	261	0.01%	0.002%
8	2.886	572	574	578	rVB2	396	239	0.01%	0.002%
9	2.912	578	582	585	rBV3	344	322	0.02%	0.002%
10	2.954	590	595	598	rBV3	462	589	0.03%	0.004%
11	3.095	636	639	642	rVB2	291	195	0.01%	0.001%
12	3.118	642	646	647	rBV	513	318	0.02%	0.002%
13	3.169	659	662	665	rBV2	489	283	0.02%	0.002%
14	3.185	665	667	669	rBV2	270	147	0.01%	0.001%
15	3.198	669	671	675	rVV2	225	134	0.01%	0.001%
16	3.240	681	684	688	rBV3	368	278	0.02%	0.002%
17	3.291	698	700	702	rVB	387	127	0.01%	0.001%
18	3.317	706	708	711	rVB2	393	190	0.01%	0.001%
19	3.333	711	713	715	rBV2	323	172	0.01%	0.001%
20	3.426	740	742	744	rBV	441	202	0.01%	0.001%
21	3.516	768	770	772	rBV	423	257	0.01%	0.002%
22	3.545	775	779	783	rVB2	365	257	0.01%	0.002%
23	3.571	783	787	790	rBV3	465	478	0.03%	0.003%
24	3.619	798	802	808	rVB2	312	336	0.02%	0.002%
25	3.648	808	811	813	rBV2	193	144	0.01%	0.001%
26	3.683	820	822	827	rBV2	428	270	0.02%	0.002%
27	3.741	838	840	842	rVB	249	105	0.01%	0.001%
28	3.767	846	848	852	rVV2	298	161	0.01%	0.001%
29	3.790	853	855	859	rVB4	421	265	0.02%	0.002%
30	3.809	859	861	862	rBV4	297	134	0.01%	0.001%
31	3.873	871	881	915	rBV	153499	411813	23.55%	2.965%
32	4.355	1013	1031	1067	rBV3	326433	1081081	61.82%	7.784%
33	4.654	1122	1124	1126	rBV2	340	106	0.01%	0.001%
34	4.706	1139	1140	1142	rBV	301	106	0.01%	0.001%
35	4.812	1171	1173	1176	rBV	400	219	0.01%	0.002%
36	4.912	1201	1204	1205	rBV	455	236	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021637.D
 Acq On : 13 Jul 2021 11:45
 Operator : SY/MD
 Sample : M3008-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.047	1229	1246	1276	rBV2	682096	1748790	100.00%	12.592%
38	5.410	1353	1359	1360	rBV3	866	740	0.04%	0.005%
39	5.465	1374	1376	1380	rVB3	339	183	0.01%	0.001%
40	5.490	1380	1384	1385	rBV3	469	328	0.02%	0.002%
41	5.545	1398	1401	1402	rBV2	547	338	0.02%	0.002%
42	5.619	1412	1424	1458	rBV	523813	1052898	60.21%	7.581%
43	5.912	1503	1515	1530	rBV3	19328	41272	2.36%	0.297%
44	6.072	1551	1565	1589	rBV	383473	786307	44.96%	5.662%
45	6.371	1656	1658	1662	rVB4	450	229	0.01%	0.002%
46	6.516	1691	1703	1717	rBV	44288	83699	4.79%	0.603%
47	6.709	1762	1763	1769	rVB2	631	452	0.03%	0.003%
48	6.751	1772	1776	1778	rBV3	468	311	0.02%	0.002%
49	6.786	1784	1787	1791	rBV3	528	431	0.02%	0.003%
50	6.825	1795	1799	1805	rVB2	581	448	0.03%	0.003%
51	6.860	1807	1810	1812	rBV2	299	151	0.01%	0.001%
52	6.921	1826	1829	1834	rVB3	470	294	0.02%	0.002%
53	6.989	1835	1850	1876	rBV	233814	426478	24.39%	3.071%
54	7.317	1940	1952	1971	rBV	838433	1455424	83.22%	10.480%
55	7.625	2038	2048	2077	rBV	158238	276218	15.79%	1.989%
56	7.834	2111	2113	2114	rBV	371	119	0.01%	0.001%
57	7.895	2127	2132	2134	rBV2	298	268	0.02%	0.002%
58	7.908	2134	2136	2138	rBV2	276	130	0.01%	0.001%
59	7.995	2161	2163	2167	rVB3	521	292	0.02%	0.002%
60	8.024	2170	2172	2174	rBV3	345	201	0.01%	0.001%
61	8.088	2182	2192	2225	rBV	476371	878770	50.25%	6.328%
62	8.555	2334	2337	2341	rVB3	529	391	0.02%	0.003%
63	8.577	2341	2344	2346	rBV3	402	238	0.01%	0.002%
64	8.619	2355	2357	2359	rBV2	316	145	0.01%	0.001%
65	8.686	2376	2378	2382	rVB2	426	220	0.01%	0.002%
66	8.731	2390	2392	2396	rBV2	351	237	0.01%	0.002%
67	8.767	2401	2403	2405	rVB	379	149	0.01%	0.001%
68	8.796	2409	2412	2415	rVB2	369	215	0.01%	0.002%
69	8.854	2418	2430	2455	rBV	779691	1254443	71.73%	9.033%
70	9.236	2547	2549	2552	rBV2	747	383	0.02%	0.003%
71	9.313	2571	2573	2575	rBV	299	118	0.01%	0.001%
72	9.432	2608	2610	2613	rBV2	574	367	0.02%	0.003%
73	9.474	2621	2623	2627	rBV3	248	207	0.01%	0.001%
74	9.558	2645	2649	2652	rVB2	666	431	0.02%	0.003%
75	9.651	2677	2678	2683	rVB3	379	156	0.01%	0.001%
76	9.674	2683	2685	2686	rBV	324	164	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021637.D
 Acq On : 13 Jul 2021 11:45
 Operator : SY/MD
 Sample : M3008-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.844	2735	2738	2741	rVB	365	288	0.02%	0.002%
78	9.863	2741	2744	2745	rBV	441	225	0.01%	0.002%
79	9.902	2752	2756	2758	rBV2	514	383	0.02%	0.003%
80	9.976	2776	2779	2780	rBV	216	100	0.01%	0.001%
81	10.127	2819	2826	2839	rVB4	5513	9248	0.53%	0.067%
82	10.217	2843	2854	2877	rVV	522501	829475	47.43%	5.973%
83	10.442	2921	2924	2928	rBV2	656	479	0.03%	0.003%
84	10.551	2956	2958	2959	rBV2	637	281	0.02%	0.002%
85	10.651	2986	2989	2992	rBV2	732	594	0.03%	0.004%
86	10.696	2999	3003	3006	rBV3	404	327	0.02%	0.002%
87	10.747	3014	3019	3022	rBV2	411	418	0.02%	0.003%
88	10.921	3062	3073	3083	rVB6	4975	8296	0.47%	0.060%
89	11.146	3135	3143	3152	rBV5	3227	5239	0.30%	0.038%
90	11.252	3165	3176	3196	rBV	789460	1227018	70.16%	8.835%
91	11.548	3259	3268	3270	rBV3	2280	2848	0.16%	0.021%
92	11.625	3280	3292	3317	rBV	808316	1270803	72.67%	9.151%
93	11.934	3384	3388	3391	rVB	601	355	0.02%	0.003%
94	11.989	3400	3405	3408	rBV5	507	559	0.03%	0.004%
95	12.037	3418	3420	3421	rBV	392	196	0.01%	0.001%
96	12.101	3432	3440	3446	rBV4	1324	2151	0.12%	0.015%
97	12.342	3513	3515	3517	rBV	426	203	0.01%	0.001%
98	12.397	3531	3532	3536	rBB3	429	203	0.01%	0.001%
99	12.487	3558	3560	3562	rBV2	715	416	0.02%	0.003%
100	13.291	3807	3810	3812	rBV2	696	359	0.02%	0.003%




Sum of corrected areas: 13887796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021637.D
Acq On : 13 Jul 2021 11:45
Operator : SY/MD
Sample : M3008-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

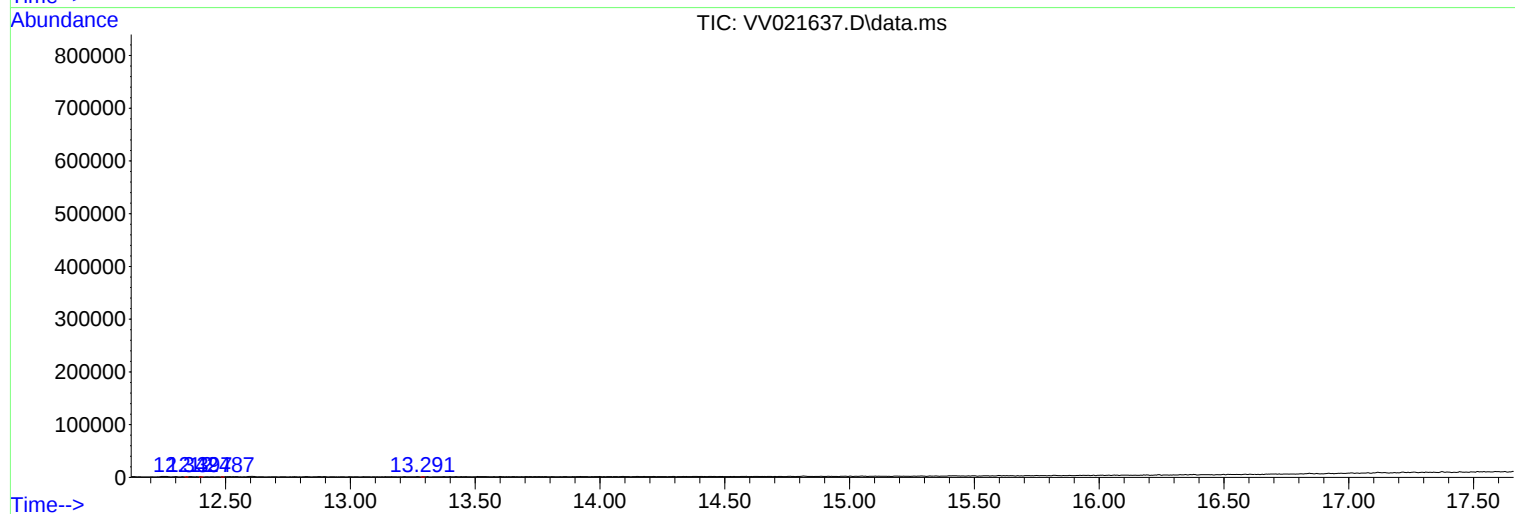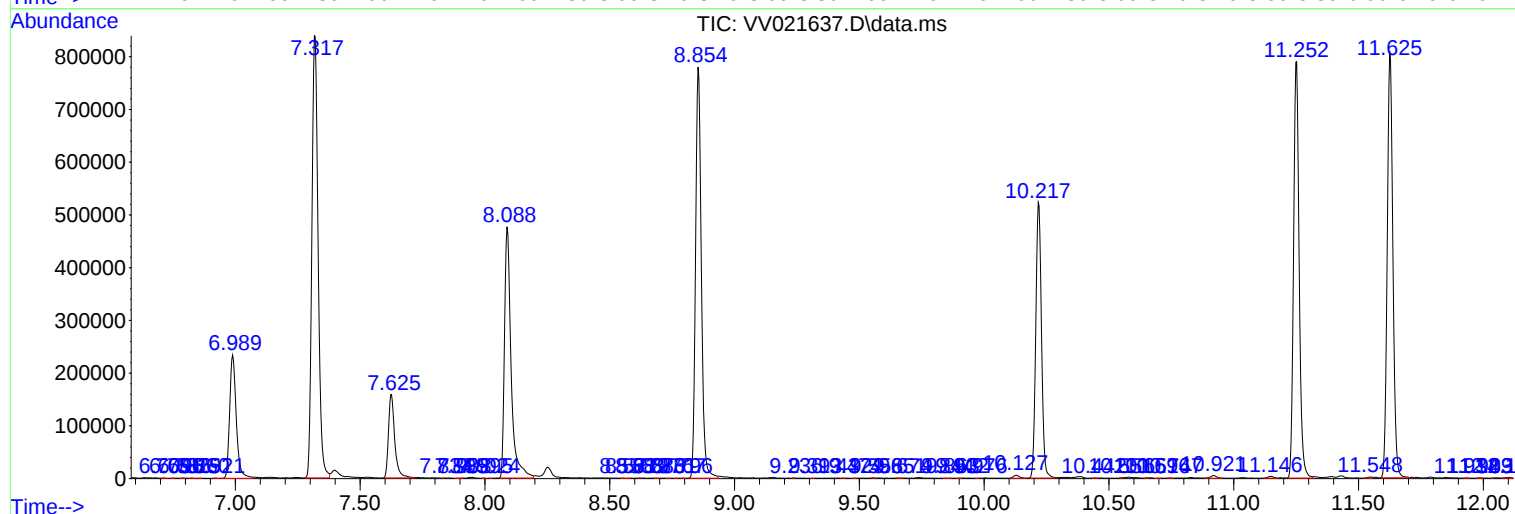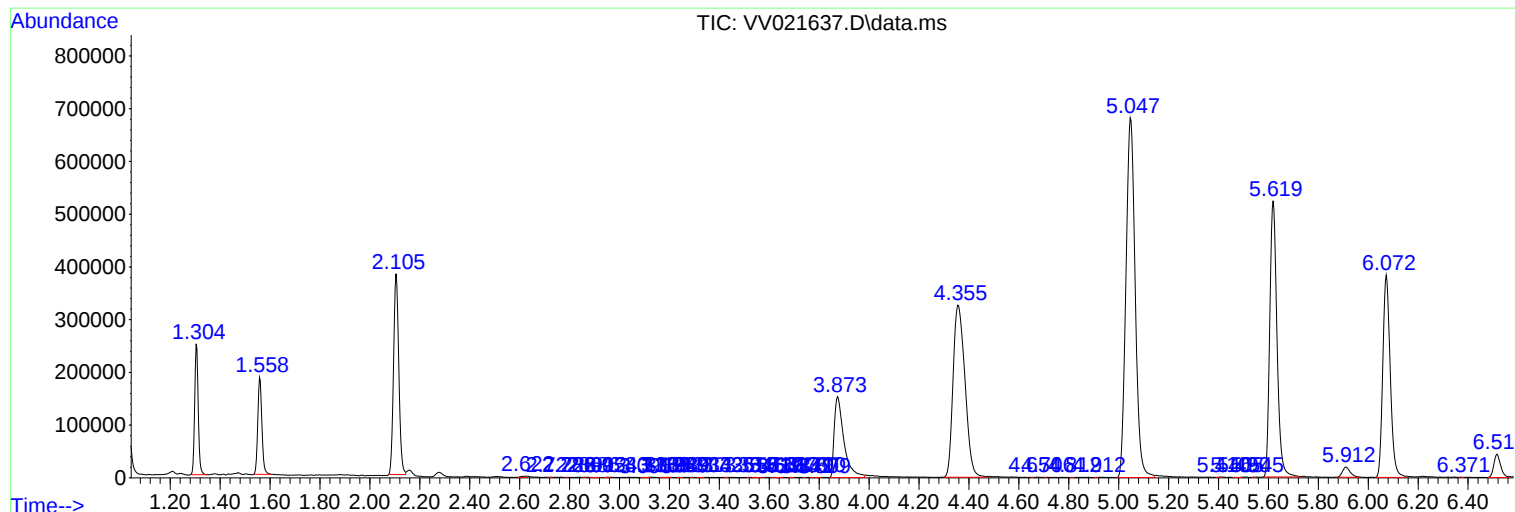

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021637.D
Acq On : 13 Jul 2021 11:45
Operator : SY/MD
Sample : M3008-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021637.D
Acq On : 13 Jul 2021 11:45
Operator : SY/MD
Sample : M3008-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
