

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021638.D
 Acq On : 13 Jul 2021 12:08
 Operator : SY/MD
 Sample : M3008-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	247732	240991	14.00%	1.765%
2	1.558	154	161	180	rVB	172287	209083	12.14%	1.531%
3	2.105	321	331	344	rBV	377324	554371	32.20%	4.060%
4	2.507	450	456	459	rBV4	1705	2171	0.13%	0.016%
5	2.590	480	482	483	rBV	585	243	0.01%	0.002%
6	2.712	518	520	523	rBV	499	302	0.02%	0.002%
7	2.735	523	527	528	rBV2	390	277	0.02%	0.002%
8	3.098	639	640	644	rVB2	444	188	0.01%	0.001%
9	3.117	644	646	649	rBV2	195	146	0.01%	0.001%
10	3.150	652	656	658	rBV2	400	224	0.01%	0.002%
11	3.394	729	732	735	rVB2	429	228	0.01%	0.002%
12	3.410	735	737	743	rVB3	444	335	0.02%	0.002%
13	3.436	743	745	747	rBV	306	147	0.01%	0.001%
14	3.490	759	762	764	rBV	357	228	0.01%	0.002%
15	3.552	778	781	782	rBV2	243	152	0.01%	0.001%
16	3.597	793	795	799	rBV2	257	201	0.01%	0.001%
17	3.625	802	804	809	rVB2	302	219	0.01%	0.002%
18	3.654	809	813	815	rBV2	285	218	0.01%	0.002%
19	3.716	830	832	836	rBV	373	299	0.02%	0.002%
20	3.777	848	851	856	rVB2	408	321	0.02%	0.002%
21	3.812	859	862	864	rBV	250	167	0.01%	0.001%
22	3.838	867	870	871	rBV	315	212	0.01%	0.002%
23	3.873	871	881	916	rBV	145360	392117	22.77%	2.871%
24	4.355	1011	1031	1065	rBV3	331628	1108156	64.36%	8.115%
25	4.629	1114	1116	1119	rBV2	417	272	0.02%	0.002%
26	4.722	1143	1145	1149	rVB	553	293	0.02%	0.002%
27	4.744	1149	1152	1154	rBV2	257	186	0.01%	0.001%
28	4.802	1169	1170	1173	rVB2	467	210	0.01%	0.002%
29	4.857	1185	1187	1190	rVB3	363	182	0.01%	0.001%
30	4.931	1208	1210	1214	rVB2	298	179	0.01%	0.001%
31	4.950	1214	1216	1220	rVB	290	179	0.01%	0.001%
32	5.047	1222	1246	1282	rBV2	668351	1721914	100.00%	12.609%
33	5.381	1347	1350	1352	rBV2	645	391	0.02%	0.003%
34	5.481	1377	1381	1382	rBV2	553	390	0.02%	0.003%
35	5.619	1411	1424	1452	rBV	512215	1028599	59.74%	7.532%
36	5.908	1504	1514	1538	rBB3	17830	40841	2.37%	0.299%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021638.D
 Acq On : 13 Jul 2021 12:08
 Operator : SY/MD
 Sample : M3008-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.072	1550	1565	1591	rBV	381790	772558	44.87%	5.657%
38	6.394	1664	1665	1666	rBV	421	158	0.01%	0.001%
39	6.436	1674	1678	1681	rBV2	417	369	0.02%	0.003%
40	6.516	1689	1703	1722	rBV	46161	90545	5.26%	0.663%
41	6.629	1736	1738	1739	rBV	401	146	0.01%	0.001%
42	6.722	1765	1767	1769	rBV	279	151	0.01%	0.001%
43	6.793	1786	1789	1790	rVV2	276	182	0.01%	0.001%
44	6.815	1794	1796	1799	rVV	310	180	0.01%	0.001%
45	6.902	1819	1823	1825	rBV2	282	206	0.01%	0.002%
46	6.915	1825	1827	1830	rVB2	506	214	0.01%	0.002%
47	6.989	1838	1850	1884	rBV	230431	423048	24.57%	3.098%
48	7.182	1908	1910	1911	rBV2	485	215	0.01%	0.002%
49	7.236	1925	1927	1928	rBV	799	358	0.02%	0.003%
50	7.320	1941	1953	1971	rBV	826318	1431580	83.14%	10.483%
51	7.625	2037	2048	2073	rBV	152380	270965	15.74%	1.984%
52	7.866	2120	2123	2126	rBV2	466	236	0.01%	0.002%
53	8.030	2171	2174	2175	rBV2	443	223	0.01%	0.002%
54	8.088	2182	2192	2232	rBV	457515	857857	49.82%	6.282%
55	8.500	2317	2320	2321	rBV	446	230	0.01%	0.002%
56	8.548	2333	2335	2337	rBV2	368	138	0.01%	0.001%
57	8.561	2337	2339	2343	rBV3	369	208	0.01%	0.002%
58	8.600	2349	2351	2354	rBV2	564	413	0.02%	0.003%
59	8.661	2366	2370	2372	rVB2	228	152	0.01%	0.001%
60	8.686	2375	2378	2385	rVB3	621	523	0.03%	0.004%
61	8.725	2385	2390	2391	rBV2	326	283	0.02%	0.002%
62	8.799	2410	2413	2416	rVB2	467	288	0.02%	0.002%
63	8.854	2416	2430	2456	rBV	750716	1232148	71.56%	9.023%
64	9.156	2518	2524	2529	rVB6	1209	1640	0.10%	0.012%
65	9.217	2541	2543	2544	rBV6	397	185	0.01%	0.001%
66	9.236	2547	2549	2552	rVV2	567	365	0.02%	0.003%
67	9.268	2556	2559	2562	rVB2	251	153	0.01%	0.001%
68	9.288	2562	2565	2566	rBV2	333	180	0.01%	0.001%
69	9.307	2569	2571	2576	rVB	427	344	0.02%	0.003%
70	9.342	2580	2582	2586	rVB3	444	284	0.02%	0.002%
71	9.593	2658	2660	2663	rBV2	334	164	0.01%	0.001%
72	9.628	2668	2671	2672	rBV	347	205	0.01%	0.002%
73	9.680	2680	2687	2691	rBV4	859	806	0.05%	0.006%
74	9.731	2699	2703	2704	rBV2	1037	703	0.04%	0.005%
75	9.809	2723	2727	2730	rBV2	354	252	0.01%	0.002%
76	9.834	2733	2735	2737	rVB	375	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021638.D
 Acq On : 13 Jul 2021 12:08
 Operator : SY/MD
 Sample : M3008-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGE66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.886	2748	2751	2752	rBV	253	157	0.01%	0.001%
78	9.998	2783	2786	2788	rBV3	583	409	0.02%	0.003%
79	10.130	2819	2827	2836	rVB3	5763	9021	0.52%	0.066%
80	10.217	2843	2854	2876	rBV	515397	814360	47.29%	5.963%
81	10.712	3006	3008	3010	rBV2	303	182	0.01%	0.001%
82	10.921	3065	3073	3085	rVB3	4986	8288	0.48%	0.061%
83	11.034	3105	3108	3110	rBV2	986	682	0.04%	0.005%
84	11.149	3134	3144	3152	rVB5	2841	4864	0.28%	0.036%
85	11.181	3152	3154	3155	rBV	546	262	0.02%	0.002%
86	11.252	3164	3176	3196	rBV	748008	1182302	68.66%	8.658%
87	11.625	3281	3292	3315	rBV	775703	1236876	71.83%	9.057%
88	11.921	3381	3384	3390	rVB2	519	496	0.03%	0.004%
89	11.982	3398	3403	3405	rBV	474	436	0.03%	0.003%
90	12.201	3468	3471	3474	rBV3	391	261	0.02%	0.002%
91	12.423	3538	3540	3545	rVB2	423	302	0.02%	0.002%
92	12.452	3545	3549	3553	rBV3	835	653	0.04%	0.005%
93	12.580	3585	3589	3590	rBV	397	284	0.02%	0.002%
94	12.596	3591	3594	3597	rBV3	900	709	0.04%	0.005%
95	12.654	3610	3612	3615	rBV	580	354	0.02%	0.003%
96	12.722	3629	3633	3639	rBV2	503	524	0.03%	0.004%
97	12.882	3680	3683	3684	rBV2	576	234	0.01%	0.002%
98	12.950	3701	3704	3705	rBV2	383	166	0.01%	0.001%
99	13.114	3753	3755	3756	rBV2	410	187	0.01%	0.001%
100	13.323	3818	3820	3823	rBV3	507	220	0.01%	0.002%




Sum of corrected areas: 13655875

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021638.D
Acq On : 13 Jul 2021 12:08
Operator : SY/MD
Sample : M3008-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

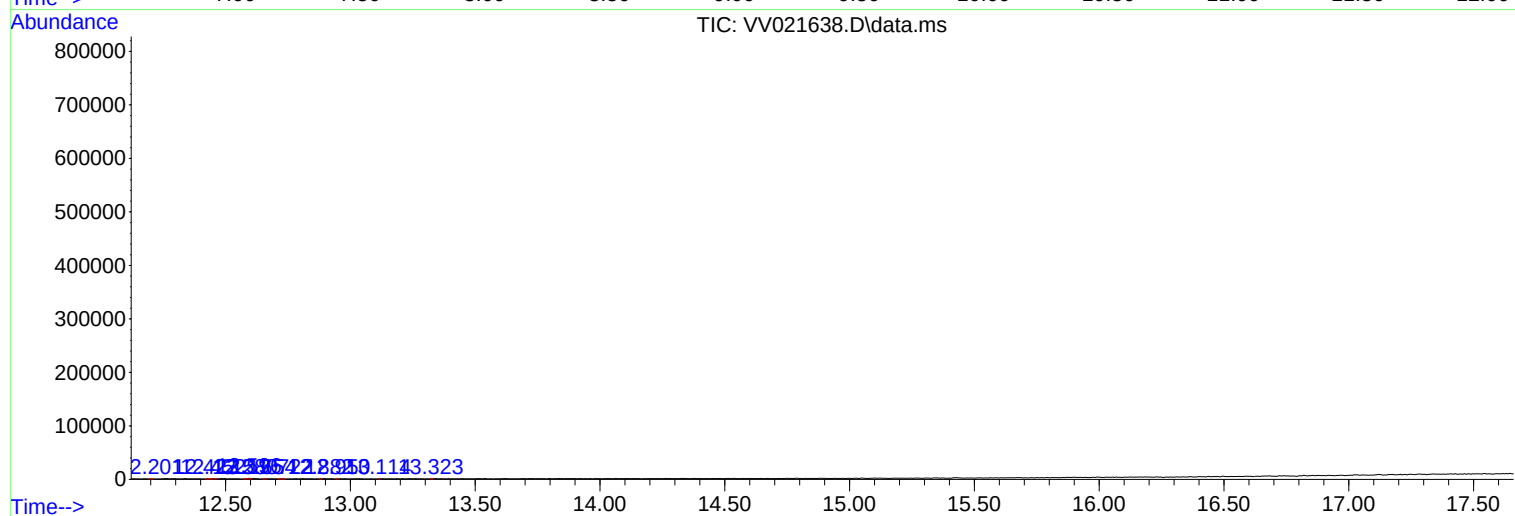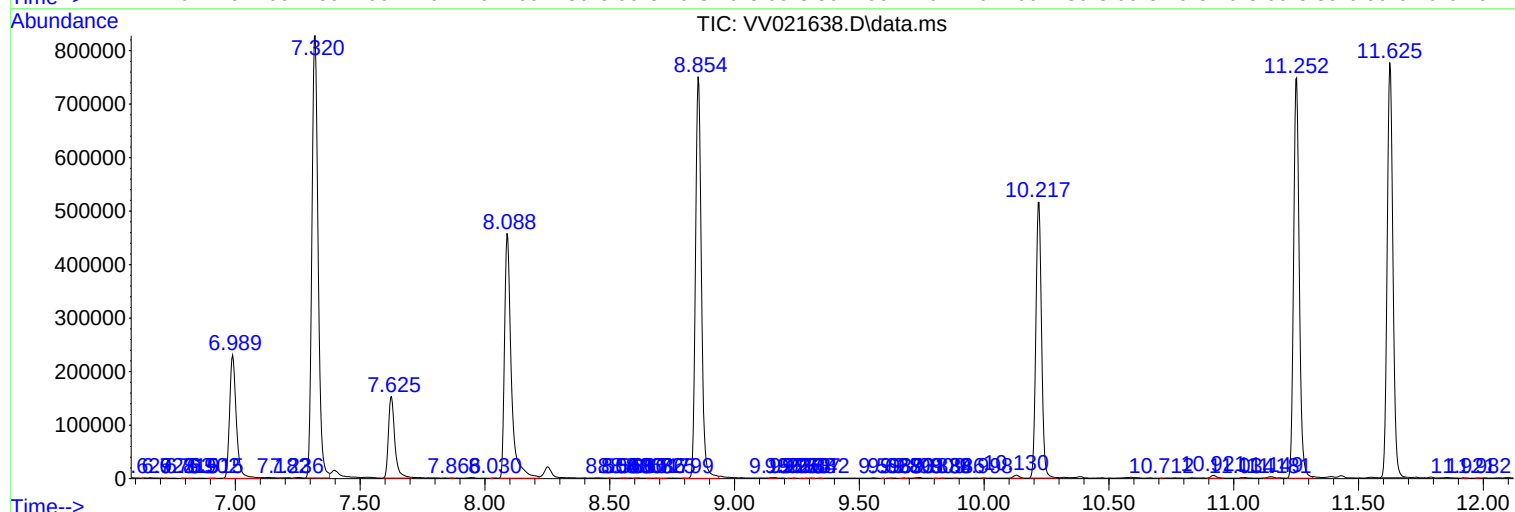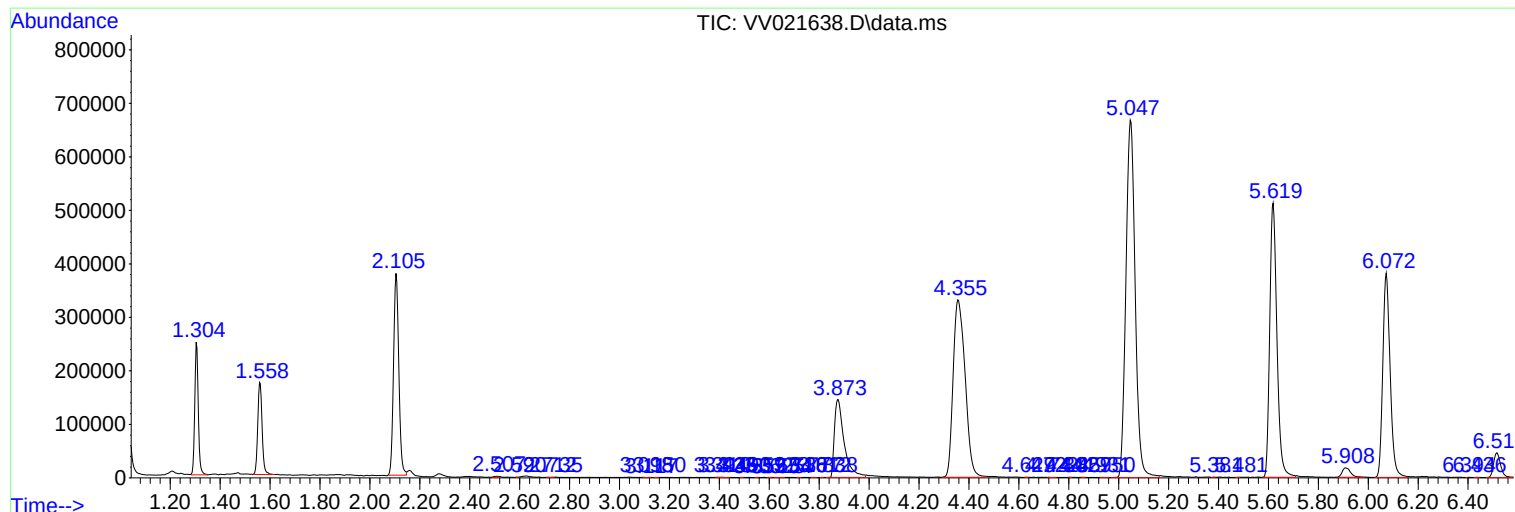

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021638.D
Acq On : 13 Jul 2021 12:08
Operator : SY/MD
Sample : M3008-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021638.D
Acq On : 13 Jul 2021 12:08
Operator : SY/MD
Sample : M3008-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGE66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
