

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021641.D
 Acq On : 13 Jul 2021 13:20
 Operator : SY/MD
 Sample : M2959-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	256357	249336	14.07%	1.817%
2	1.558	154	161	177	rVB	186279	215861	12.18%	1.573%
3	2.104	321	331	358	rVB	394245	583890	32.96%	4.255%
4	2.503	448	455	468	rVB3	6175	11128	0.63%	0.081%
5	2.555	469	471	475	rVB4	374	256	0.01%	0.002%
6	2.767	534	537	540	rVB3	582	279	0.02%	0.002%
7	2.825	553	555	558	rBV	240	154	0.01%	0.001%
8	2.921	583	585	588	rVB3	301	154	0.01%	0.001%
9	3.040	616	622	623	rBV3	912	856	0.05%	0.006%
10	3.130	648	650	654	rVB3	447	222	0.01%	0.002%
11	3.153	654	657	660	rBV2	242	176	0.01%	0.001%
12	3.204	670	673	676	rVB3	389	200	0.01%	0.001%
13	3.330	710	712	715	rVB	304	159	0.01%	0.001%
14	3.448	743	749	753	rBV2	328	347	0.02%	0.003%
15	3.484	757	760	762	rBV	242	167	0.01%	0.001%
16	3.535	773	776	778	rBV2	318	194	0.01%	0.001%
17	3.577	785	789	791	rBV	367	176	0.01%	0.001%
18	3.625	802	804	806	rBV2	276	158	0.01%	0.001%
19	3.715	827	832	835	rBV3	453	463	0.03%	0.003%
20	3.764	843	847	848	rBV	240	169	0.01%	0.001%
21	3.796	853	857	859	rBV2	273	199	0.01%	0.001%
22	3.873	870	881	914	rBV	160149	415452	23.45%	3.027%
23	4.349	1011	1029	1065	rBV	277422	692873	39.11%	5.049%
24	4.870	1189	1191	1195	rVB3	472	296	0.02%	0.002%
25	4.892	1195	1198	1200	rBV	537	317	0.02%	0.002%
26	4.908	1200	1203	1204	rBV	300	135	0.01%	0.001%
27	5.046	1228	1246	1272	rBV2	694214	1771647	100.00%	12.910%
28	5.493	1383	1385	1388	rVB	416	171	0.01%	0.001%
29	5.548	1399	1402	1406	rVB2	405	293	0.02%	0.002%
30	5.616	1411	1423	1458	rVV	538977	1089127	61.48%	7.936%
31	5.908	1503	1514	1535	rVB2	16379	36180	2.04%	0.264%
32	6.021	1546	1549	1551	rBV2	303	228	0.01%	0.002%
33	6.072	1551	1565	1589	rBV	387683	799785	45.14%	5.828%
34	6.320	1640	1642	1644	rBV2	507	229	0.01%	0.002%
35	6.390	1656	1664	1667	rBV6	474	479	0.03%	0.003%
36	6.435	1676	1678	1681	rBV	315	187	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071321\
 Data File : VW021641.D
 Acq On : 13 Jul 2021 13:20
 Operator : SY/MD
 Sample : M2959-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.461	1681	1686	1688	rBV2	235	201	0.01%	0.001%
38	6.503	1693	1699	1701	rBV3	501	501	0.03%	0.004%
39	6.532	1705	1708	1714	rVB4	401	436	0.02%	0.003%
40	6.641	1736	1742	1747	rBV3	1037	1615	0.09%	0.012%
41	6.689	1756	1757	1761	rVV3	301	163	0.01%	0.001%
42	6.718	1764	1766	1770	rVB2	423	214	0.01%	0.002%
43	6.770	1780	1782	1784	rBV2	404	179	0.01%	0.001%
44	6.834	1800	1802	1806	rVV3	276	203	0.01%	0.001%
45	6.924	1828	1830	1832	rVB	418	189	0.01%	0.001%
46	6.989	1838	1850	1871	rBV	237388	428693	24.20%	3.124%
47	7.210	1915	1919	1928	rVB	9167	6681	0.38%	0.049%
48	7.316	1939	1952	1970	rBV	849525	1477183	83.38%	10.764%
49	7.625	2038	2048	2072	rBV	163587	278821	15.74%	2.032%
50	7.860	2118	2121	2124	rBV2	508	389	0.02%	0.003%
51	7.876	2124	2126	2129	rVB3	391	177	0.01%	0.001%
52	7.895	2129	2132	2133	rBV	554	262	0.01%	0.002%
53	7.995	2162	2163	2168	rVB2	181	132	0.01%	0.001%
54	8.024	2169	2172	2175	rVB2	381	223	0.01%	0.002%
55	8.040	2175	2177	2179	rVB	318	132	0.01%	0.001%
56	8.088	2182	2192	2225	rBV	488862	903350	50.99%	6.583%
57	8.442	2298	2302	2306	rVB3	642	458	0.03%	0.003%
58	8.474	2310	2312	2313	rBV	339	151	0.01%	0.001%
59	8.535	2328	2331	2334	rBV2	366	293	0.02%	0.002%
60	8.570	2338	2342	2347	rBV2	507	449	0.03%	0.003%
61	8.603	2350	2352	2356	rBV2	642	342	0.02%	0.002%
62	8.686	2376	2378	2380	rBV2	286	144	0.01%	0.001%
63	8.702	2380	2383	2385	rVV2	263	131	0.01%	0.001%
64	8.802	2413	2414	2419	rBV2	233	134	0.01%	0.001%
65	8.853	2419	2430	2449	rBV	792236	1286619	72.62%	9.376%
66	9.101	2505	2507	2511	rBV3	285	188	0.01%	0.001%
67	9.246	2550	2552	2554	rBV2	535	274	0.02%	0.002%
68	9.336	2576	2580	2581	rBV	321	266	0.02%	0.002%
69	9.374	2590	2592	2595	rBV	235	167	0.01%	0.001%
70	9.390	2595	2597	2600	rVV2	268	167	0.01%	0.001%
71	9.435	2609	2611	2614	rVB2	286	152	0.01%	0.001%
72	9.500	2627	2631	2633	rBV3	271	232	0.01%	0.002%
73	9.670	2681	2684	2688	rBV2	818	615	0.03%	0.004%
74	9.722	2698	2700	2703	rBV	293	183	0.01%	0.001%
75	9.747	2706	2708	2711	rBV2	191	159	0.01%	0.001%
76	9.831	2731	2734	2736	rBV	279	155	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021641.D
 Acq On : 13 Jul 2021 13:20
 Operator : SY/MD
 Sample : M2959-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.998	2783	2786	2790	rBV	315	230	0.01%	0.002%
78	10.024	2790	2794	2798	rVV2	353	308	0.02%	0.002%
79	10.130	2819	2827	2837	rVB2	5373	8579	0.48%	0.063%
80	10.217	2842	2854	2875	rBV	539814	854222	48.22%	6.225%
81	10.548	2952	2957	2958	rBV2	791	677	0.04%	0.005%
82	10.580	2961	2967	2972	rVV2	1258	1723	0.10%	0.013%
83	10.821	3039	3042	3044	rBV2	722	408	0.02%	0.003%
84	10.857	3051	3053	3057	rVB4	899	388	0.02%	0.003%
85	10.918	3065	3072	3084	rVB2	5633	8423	0.48%	0.061%
86	11.001	3095	3098	3101	rVB2	411	255	0.01%	0.002%
87	11.033	3101	3108	3113	rBV6	1266	1652	0.09%	0.012%
88	11.149	3131	3144	3153	rBV7	2917	5413	0.31%	0.039%
89	11.252	3164	3176	3197	rBV	818403	1275210	71.98%	9.292%
90	11.381	3211	3216	3217	rBV4	2171	1637	0.09%	0.012%
91	11.429	3226	3231	3232	rBV3	2898	2563	0.14%	0.019%
92	11.529	3260	3262	3263	rBV	459	182	0.01%	0.001%
93	11.625	3280	3292	3314	rBV	817085	1295977	73.15%	9.444%
94	11.837	3355	3358	3359	rBV2	589	319	0.02%	0.002%
95	11.975	3398	3401	3404	rVB3	490	265	0.01%	0.002%
96	11.995	3404	3407	3410	rBV2	611	463	0.03%	0.003%
97	12.165	3457	3460	3461	rBV	268	152	0.01%	0.001%
98	12.432	3539	3543	3547	rBV3	750	620	0.03%	0.005%
99	12.815	3660	3662	3664	rBV	351	178	0.01%	0.001%
100	13.397	3841	3843	3849	rVB2	531	304	0.02%	0.002%




Sum of corrected areas: 13723114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021641.D
Acq On : 13 Jul 2021 13:20
Operator : SY/MD
Sample : M2959-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

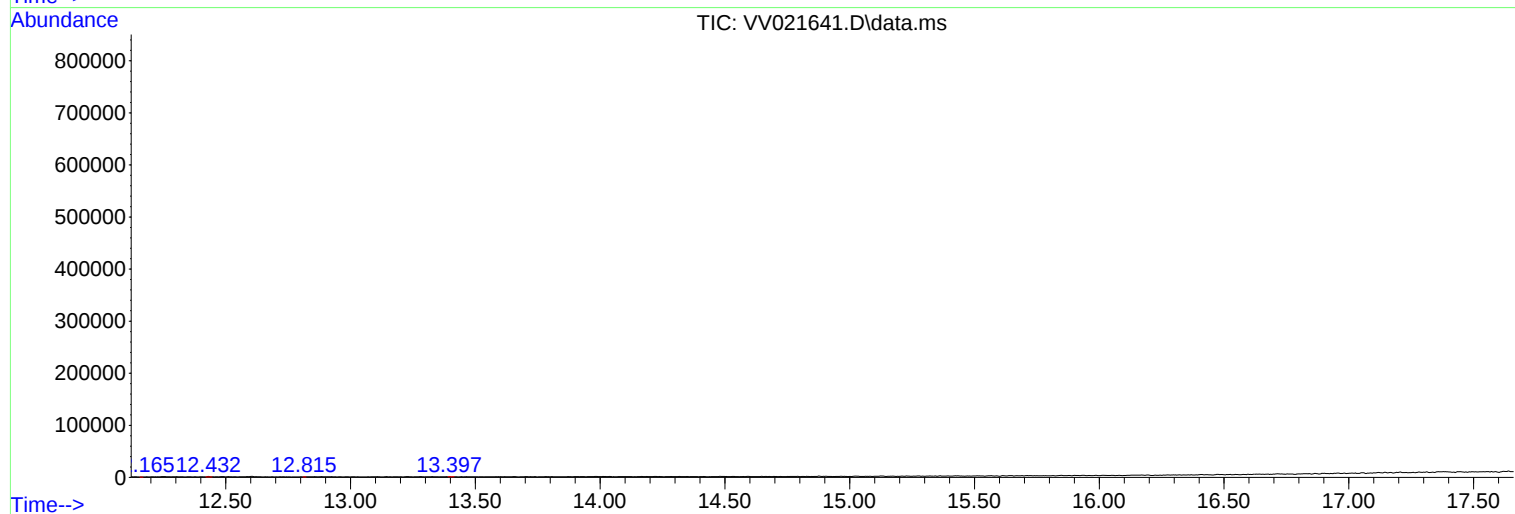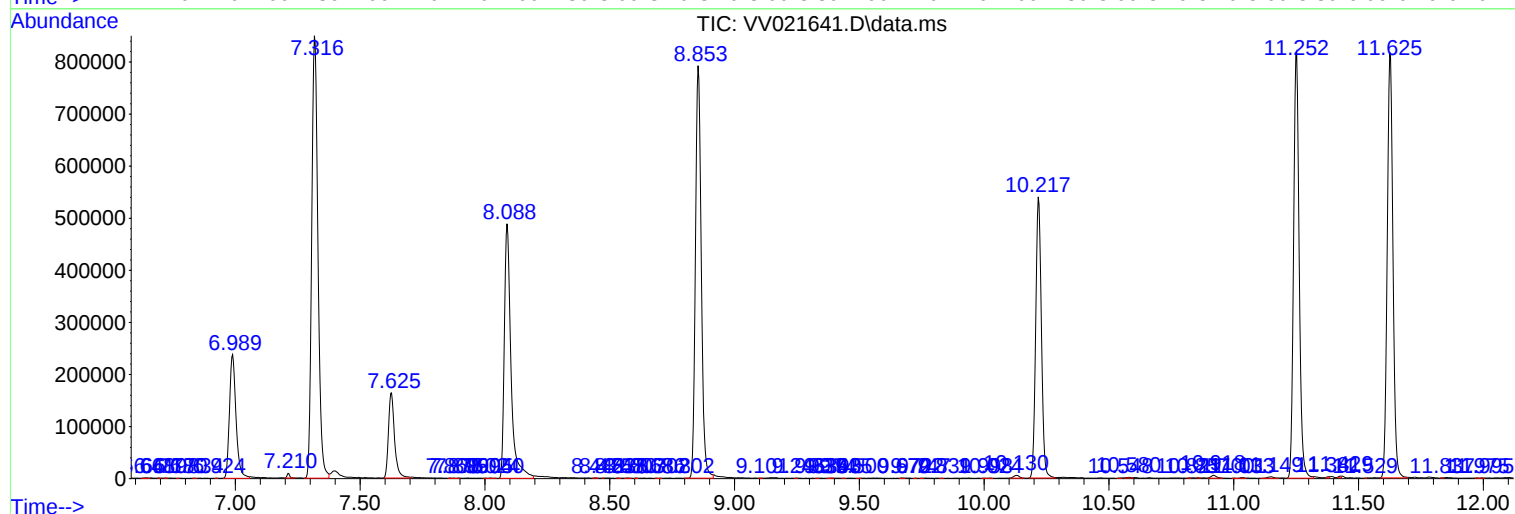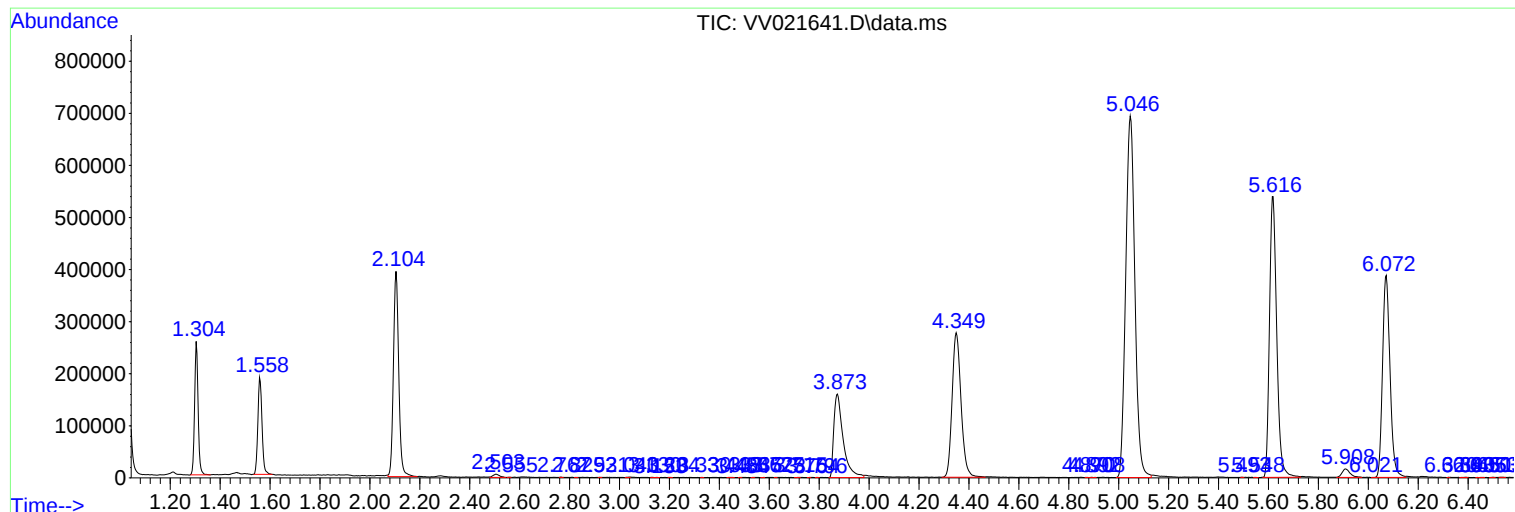

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021641.D
Acq On : 13 Jul 2021 13:20
Operator : SY/MD
Sample : M2959-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021641.D
Acq On : 13 Jul 2021 13:20
Operator : SY/MD
Sample : M2959-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
