

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021643.D
 Acq On : 13 Jul 2021 14:08
 Operator : SY/MD
 Sample : M3008-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	223441	218076	13.25%	1.715%
2	1.561	155	162	179	rVB	166506	195236	11.86%	1.536%
3	2.105	322	331	354	rVB	347800	515418	31.32%	4.054%
4	2.506	448	456	468	rVB2	7219	12492	0.76%	0.098%
5	2.613	486	489	490	rBV	571	349	0.02%	0.003%
6	2.661	501	504	505	rBV2	343	220	0.01%	0.002%
7	2.883	568	573	579	rVB3	474	429	0.03%	0.003%
8	3.011	609	613	614	rBV3	196	126	0.01%	0.001%
9	3.072	630	632	635	rVB2	423	219	0.01%	0.002%
10	3.121	644	647	648	rBV	339	188	0.01%	0.001%
11	3.178	661	665	666	rBV	356	208	0.01%	0.002%
12	3.233	680	682	685	rVB2	343	153	0.01%	0.001%
13	3.352	715	719	720	rBV2	220	149	0.01%	0.001%
14	3.365	720	723	727	rVB	373	234	0.01%	0.002%
15	3.490	757	762	764	rBV3	369	334	0.02%	0.003%
16	3.606	793	798	801	rBV2	262	230	0.01%	0.002%
17	3.738	836	839	842	rVB2	371	183	0.01%	0.001%
18	3.780	850	852	854	rBV2	395	177	0.01%	0.001%
19	3.818	861	864	868	rVB3	323	221	0.01%	0.002%
20	3.873	870	881	918	rBV	153100	407168	24.74%	3.202%
21	4.349	1012	1029	1055	rBV	254265	633108	38.47%	4.979%
22	4.555	1092	1093	1095	rBV2	367	145	0.01%	0.001%
23	4.567	1095	1097	1102	rVV2	446	343	0.02%	0.003%
24	4.783	1158	1164	1165	rBV	457	424	0.03%	0.003%
25	4.870	1188	1191	1193	rBV2	436	277	0.02%	0.002%
26	4.973	1219	1223	1224	rBV	361	165	0.01%	0.001%
27	5.047	1228	1246	1281	rBV2	639826	1645749	100.00%	12.944%
28	5.329	1331	1334	1336	rBV3	440	377	0.02%	0.003%
29	5.407	1356	1358	1363	rBV2	419	319	0.02%	0.003%
30	5.468	1374	1377	1378	rBV	397	234	0.01%	0.002%
31	5.510	1387	1390	1391	rBV	343	197	0.01%	0.002%
32	5.545	1398	1401	1404	rVB	410	228	0.01%	0.002%
33	5.564	1405	1407	1410	rVB	426	213	0.01%	0.002%
34	5.619	1410	1424	1461	rBV	487593	994341	60.42%	7.821%
35	5.908	1503	1514	1528	rBV3	15378	31798	1.93%	0.250%
36	6.072	1550	1565	1588	rBV	365729	744787	45.26%	5.858%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021643.D
 Acq On : 13 Jul 2021 14:08
 Operator : SY/MD
 Sample : M3008-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.339	1646	1648	1649	rBV	380	160	0.01%	0.001%
38	6.374	1657	1659	1662	rVB2	466	252	0.02%	0.002%
39	6.400	1665	1667	1669	rVV3	611	310	0.02%	0.002%
40	6.423	1672	1674	1675	rBV3	347	143	0.01%	0.001%
41	6.474	1687	1690	1697	rBV2	423	277	0.02%	0.002%
42	6.506	1697	1700	1703	rBV	377	325	0.02%	0.003%
43	6.696	1758	1759	1768	rVB6	515	440	0.03%	0.003%
44	6.805	1791	1793	1796	rBV2	343	279	0.02%	0.002%
45	6.854	1805	1808	1810	rBV2	377	233	0.01%	0.002%
46	6.886	1816	1818	1820	rVB2	365	124	0.01%	0.001%
47	6.902	1820	1823	1825	rBV2	289	174	0.01%	0.001%
48	6.989	1838	1850	1879	rBV	220605	404659	24.59%	3.183%
49	7.317	1940	1952	1971	rBV	781319	1357471	82.48%	10.677%
50	7.622	2038	2047	2078	rBV	152313	261949	15.92%	2.060%
51	7.879	2125	2127	2132	rVB	399	266	0.02%	0.002%
52	7.905	2133	2135	2139	rVB3	303	158	0.01%	0.001%
53	7.931	2139	2143	2145	rBV3	464	328	0.02%	0.003%
54	8.011	2165	2168	2173	rVB2	358	317	0.02%	0.002%
55	8.040	2173	2177	2179	rBV	417	256	0.02%	0.002%
56	8.088	2181	2192	2237	rBV	469602	877604	53.33%	6.902%
57	8.429	2295	2298	2301	rBV2	621	419	0.03%	0.003%
58	8.535	2326	2331	2332	rBV3	657	446	0.03%	0.004%
59	8.561	2337	2339	2341	rVB3	410	148	0.01%	0.001%
60	8.728	2387	2391	2392	rBV2	306	220	0.01%	0.002%
61	8.853	2418	2430	2459	rBV	735588	1193637	72.53%	9.388%
62	9.079	2497	2500	2505	rBV5	517	429	0.03%	0.003%
63	9.120	2510	2513	2515	rVB2	203	120	0.01%	0.001%
64	9.140	2515	2519	2521	rBV2	955	644	0.04%	0.005%
65	9.378	2590	2593	2594	rBV	217	132	0.01%	0.001%
66	9.445	2610	2614	2616	rVB2	471	267	0.02%	0.002%
67	9.487	2625	2627	2630	rVB2	400	220	0.01%	0.002%
68	9.525	2635	2639	2641	rBV	438	285	0.02%	0.002%
69	9.554	2645	2648	2650	rBV2	369	248	0.02%	0.002%
70	9.654	2676	2679	2681	rBV2	384	197	0.01%	0.002%
71	9.677	2683	2686	2688	rBV3	509	308	0.02%	0.002%
72	9.718	2695	2699	2701	rBV	350	287	0.02%	0.002%
73	9.776	2715	2717	2719	rBV2	340	122	0.01%	0.001%
74	9.802	2721	2725	2727	rBV	496	323	0.02%	0.003%
75	9.889	2749	2752	2754	rBV	298	167	0.01%	0.001%
76	9.911	2757	2759	2761	rBV	302	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
 Data File : VV021643.D
 Acq On : 13 Jul 2021 14:08
 Operator : SY/MD
 Sample : M3008-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.963	2773	2775	2777	rBV	237	122	0.01%	0.001%
78	10.040	2797	2799	2804	rVB	247	182	0.01%	0.001%
79	10.066	2804	2807	2809	rBV2	450	316	0.02%	0.002%
80	10.130	2819	2827	2835	rBV4	4902	7154	0.43%	0.056%
81	10.217	2842	2854	2875	rBV	518341	819073	49.77%	6.442%
82	10.416	2912	2916	2918	rBV2	300	211	0.01%	0.002%
83	10.519	2945	2948	2951	rBV	358	174	0.01%	0.001%
84	10.538	2952	2954	2955	rBV	375	158	0.01%	0.001%
85	10.574	2959	2965	2966	rBV	1131	1168	0.07%	0.009%
86	10.722	3008	3011	3016	rBV2	334	272	0.02%	0.002%
87	11.149	3136	3144	3146	rBV5	2275	2883	0.18%	0.023%
88	11.197	3153	3159	3161	rBV4	691	664	0.04%	0.005%
89	11.249	3164	3175	3193	rBV	744320	1169109	71.04%	9.195%
90	11.496	3250	3252	3255	rVB2	487	258	0.02%	0.002%
91	11.516	3255	3258	3260	rBV2	404	251	0.02%	0.002%
92	11.532	3260	3263	3265	rBV	390	251	0.02%	0.002%
93	11.625	3280	3292	3316	rBV	757454	1199773	72.90%	9.436%
94	11.889	3372	3374	3378	rVB4	662	337	0.02%	0.003%
95	11.982	3400	3403	3406	rVB	530	292	0.02%	0.002%
96	12.027	3414	3417	3420	rVB2	649	373	0.02%	0.003%
97	12.046	3420	3423	3430	rBV5	678	841	0.05%	0.007%
98	12.249	3483	3486	3495	rVB3	905	945	0.06%	0.007%
99	12.940	3698	3701	3703	rBV	317	253	0.02%	0.002%
100	13.371	3834	3835	3840	rVB	672	276	0.02%	0.002%




Sum of corrected areas: 12714367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021643.D
Acq On : 13 Jul 2021 14:08
Operator : SY/MD
Sample : M3008-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

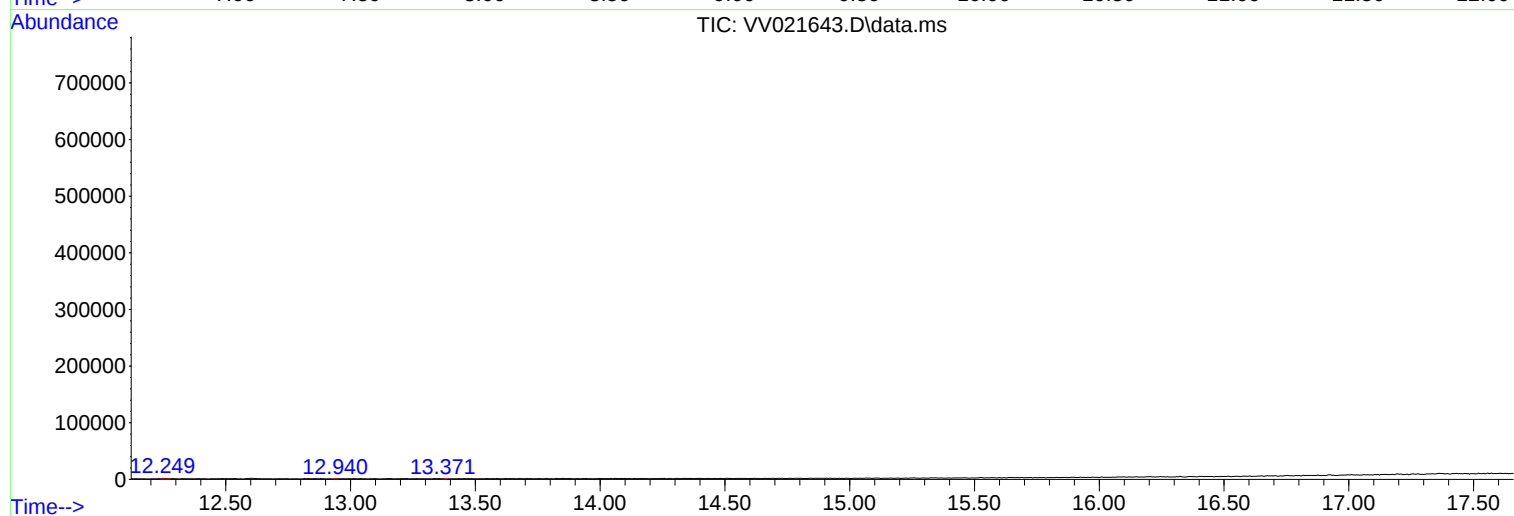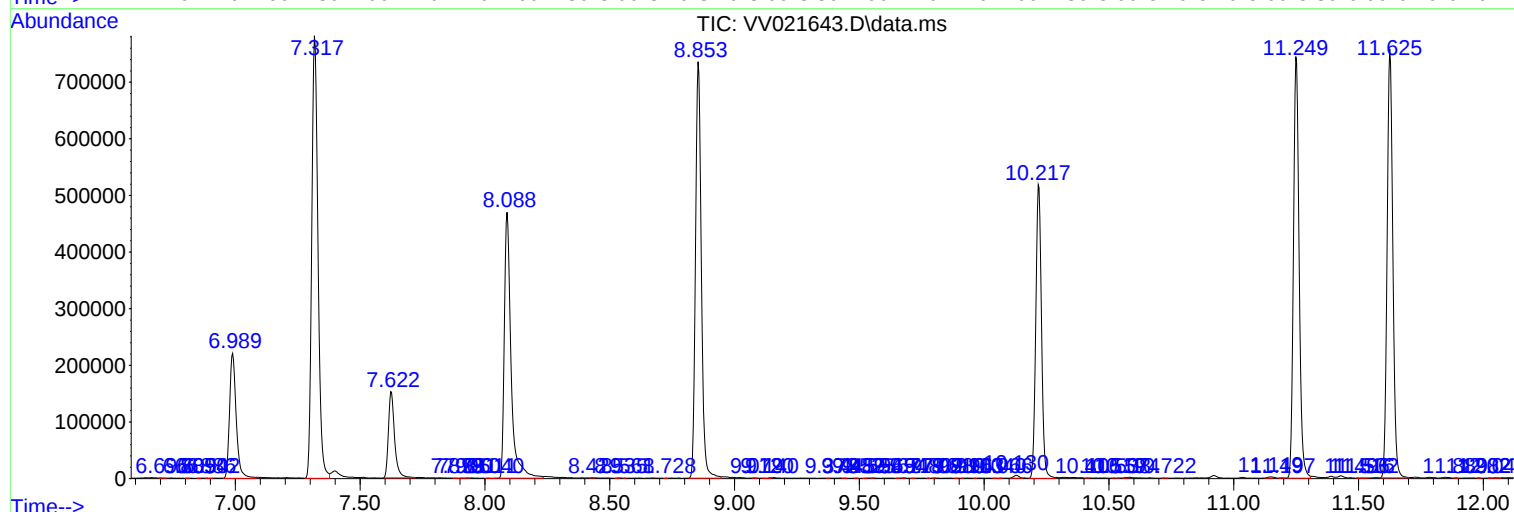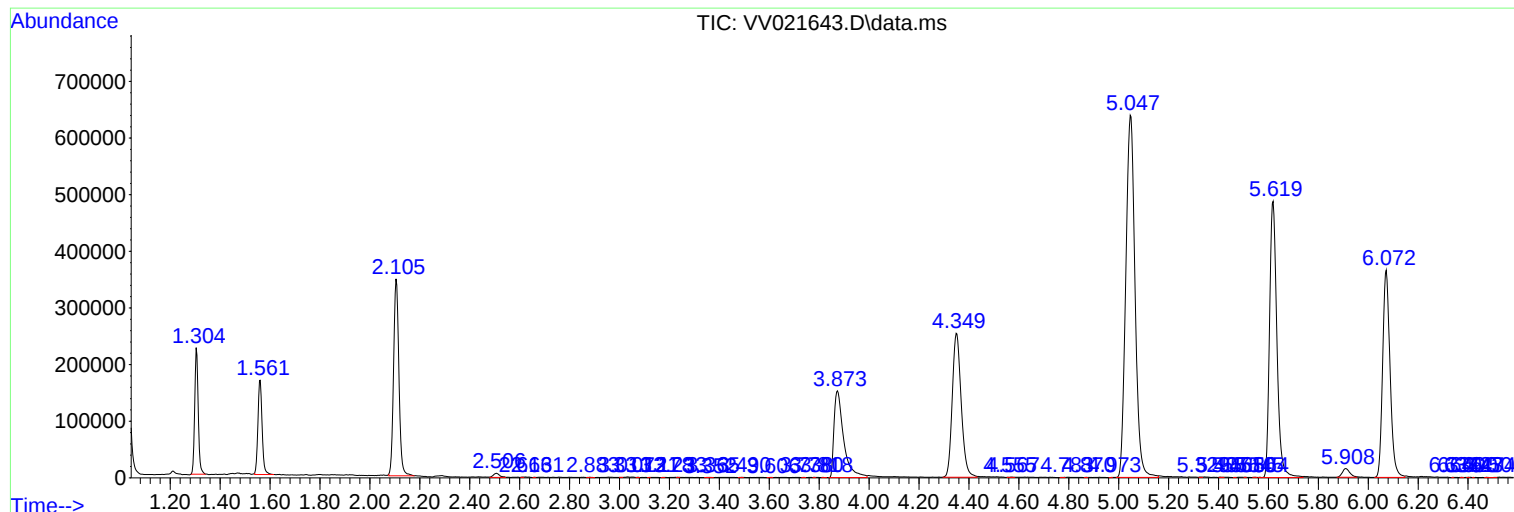

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021643.D
Acq On : 13 Jul 2021 14:08
Operator : SY/MD
Sample : M3008-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021643.D
Acq On : 13 Jul 2021 14:08
Operator : SY/MD
Sample : M3008-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
