
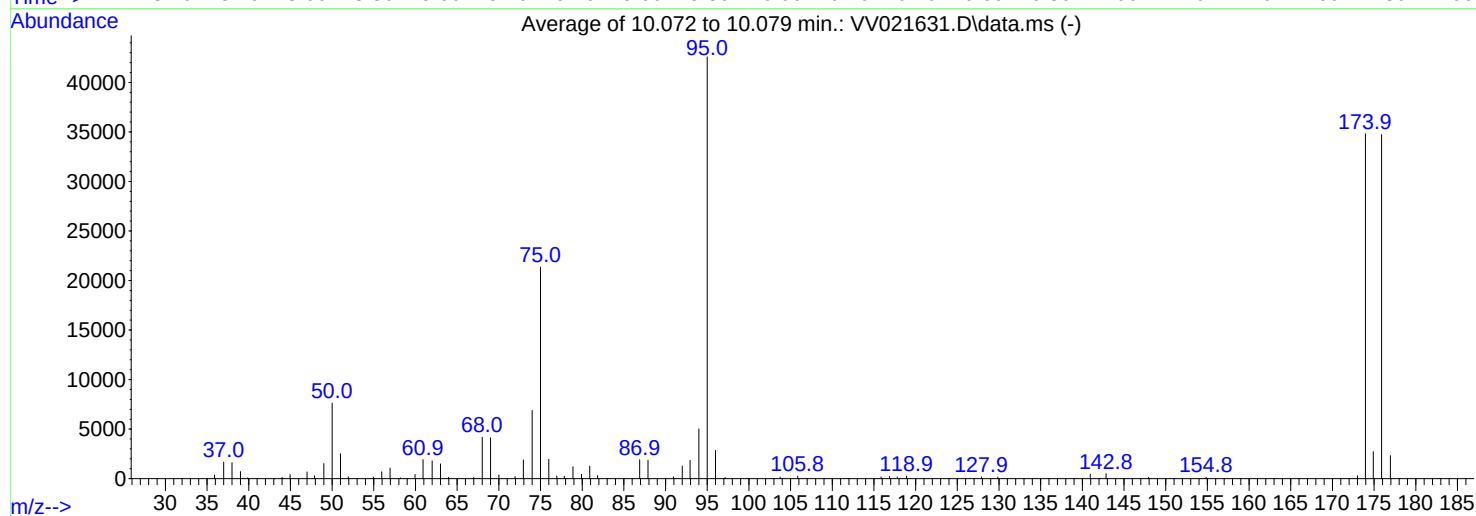


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071321\
Data File : VV021631.D
Acq On : 13 Jul 2021 09:01
Operator : SY/MD
Sample : BFB204
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB204

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Title : VOC Analysis
Last Update : Fri Jul 16 01:06:31 2021

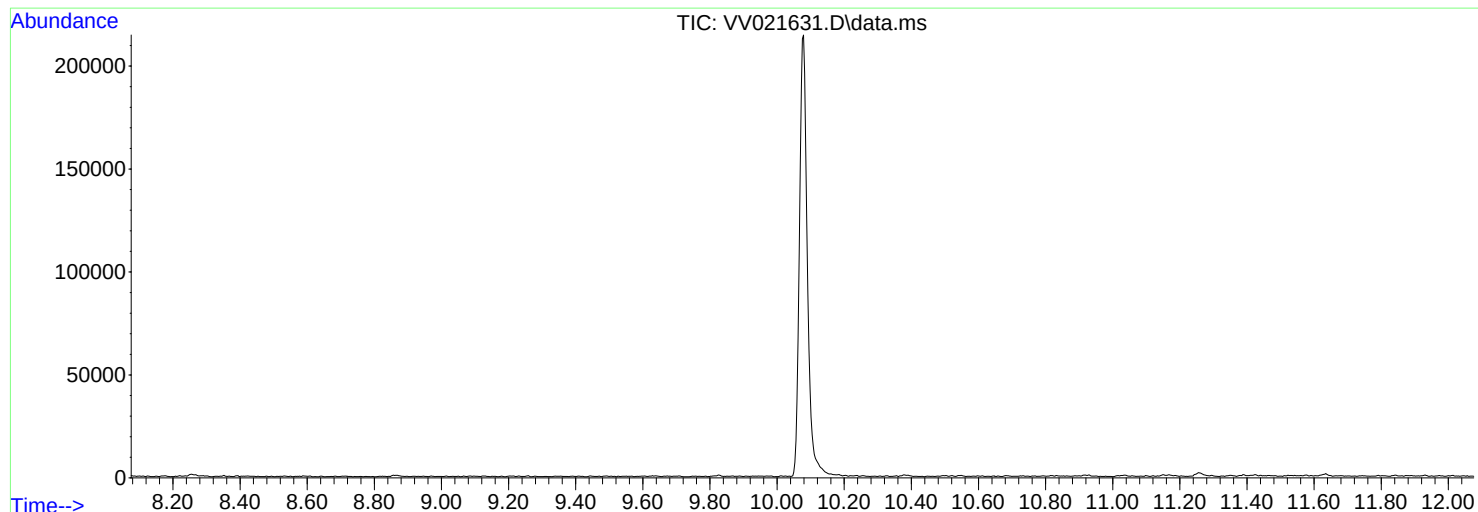

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7627	PASS
75	95	30	80	50.2	21363	PASS
95	95	100	100	100.0	42581	PASS
96	95	5	9	6.7	2838	PASS
173	174	0.00	2	0.9	296	PASS
174	95	50	120	81.8	34811	PASS
175	174	5	9	7.9	2735	PASS
176	174	95	105	99.8	34733	PASS
177	176	5	10	6.7	2333	PASS

m/z	Abundance
35.90	357.0
37.00	1736.0
38.00	1643.0
39.00	717.0
39.90	299.0
43.10	113.0
44.00	539.0
45.00	417.0
47.00	708.0
47.90	289.0
49.00	1609.0
50.00	7922.0
51.00	2613.0
52.00	195.0
54.90	153.0
55.90	730.0
57.00	1115.0
58.20	121.0
59.90	414.0
60.90	1981.0
62.00	1847.0
63.00	1556.0
63.90	142.0
67.00	145.0
68.00	4292.0
69.00	4309.0
70.00	396.0
72.00	195.0
72.90	1931.0
74.00	7110.0
75.00	22024.0
76.00	2042.0
77.00	274.0
77.90	269.0
78.90	1247.0
79.90	435.0
80.90	1269.0
81.90	308.0
86.90	1960.0
87.90	1953.0
91.00	190.0
92.00	1315.0
92.90	1932.0
94.00	5166.0
95.00	44024.0
96.00	2949.0
97.20	118.0
103.70	162.0
105.80	271.0
115.80	193.0
116.90	228.0
117.80	171.0
118.90	261.0
127.90	185.0
129.80	160.0
141.00	468.0
142.90	517.0
148.00	137.0
154.90	141.0
173.00	301.0
173.90	35832.0
174.90	2794.0
175.90	35912.0
176.90	2447.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.90	393.0
37.00	1685.0
38.00	1634.0
39.00	688.0
39.90	267.0
43.00	103.0
44.00	571.0
45.00	418.0
47.00	686.0
47.90	259.0
49.00	1479.0
50.00	7634.0
51.00	2501.0
52.00	162.0
54.90	154.0
56.00	770.0
57.00	1023.0
60.00	394.0
60.90	1943.0
62.00	1833.0
63.00	1549.0
63.90	125.0
67.00	122.0
68.00	4407.0
69.00	4191.0
70.00	340.0
71.90	248.0
73.00	1905.0
74.00	7053.0
75.00	22176.0
76.00	1970.0
77.00	320.0
77.90	211.0
78.90	1220.0
79.90	375.0
80.90	1362.0
81.80	315.0
86.90	2095.0
87.90	1856.0
91.00	189.0
92.00	1282.0
93.00	2042.0
94.00	5219.0
95.00	43984.0
96.00	2790.0
97.20	104.0
103.70	164.0
105.90	234.0
115.90	177.0
116.90	232.0
117.80	178.0
118.90	264.0
127.90	184.0
129.80	182.0
140.90	439.0
142.10	107.0
142.90	495.0
148.00	106.0
154.90	136.0
173.00	311.0
174.00	37200.0
174.90	2793.0
175.90	37456.0
177.00	2393.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
39.90	207.0
43.00	117.0
44.00	414.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.90	301.0
37.00	1589.0
38.00	1583.0
39.00	725.0
39.90	300.0
43.00	148.0
44.00	529.0
44.90	361.0
47.00	646.0
47.90	306.0
49.00	1486.0
50.00	7324.0
51.00	2422.0
51.90	205.0
55.00	158.0
56.00	587.0
56.90	1059.0
58.20	105.0
59.90	444.0
60.90	1865.0
62.00	1683.0
63.00	1340.0
64.00	141.0
67.00	145.0
68.00	3806.0
69.00	3857.0
70.00	387.0
72.00	182.0
72.90	1831.0
74.00	6508.0
75.00	19888.0
76.00	1877.0
76.90	254.0
77.80	275.0
78.90	1164.0
79.90	484.0
80.90	1146.0
81.90	298.0
86.90	1671.0
87.90	1840.0
90.90	147.0
92.00	1215.0
92.90	1554.0
94.00	4674.0
95.00	39736.0
96.00	2776.0
97.10	117.0
103.80	166.0
105.80	266.0
115.80	184.0
116.80	219.0
117.80	168.0
118.90	234.0
127.90	161.0
129.90	128.0
140.90	467.0
142.80	497.0
147.90	150.0
154.80	128.0
173.00	275.0
173.90	31400.0
174.90	2619.0
175.90	30832.0
176.90	2158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204