

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
 Data File : VV026744.D
 Acq On : 13 Jul 2022 11:33
 Operator : SY/MD
 Sample : VV0713WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK393

Quant Time: Jul 13 23:00:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 13 23:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	213465	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	214571	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	87286	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	88971	4.569	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.400%
7) Chloroethane-d5	1.558	69	79566	4.729	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.600%
11) 1,1-Dichloroethene-d2	2.098	63	128273	3.431	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	3.908	46	122045	40.154	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.300%
24) Chloroform-d	4.342	84	166579	4.892	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.031	65	76219	5.124	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.400%
32) Benzene-d6	5.047	84	301739	4.628	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
36) 1,2-Dichloropropane-d6	6.069	67	96448	4.934	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.313	98	230094	3.976	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	7.625	79	26313	4.114	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%
46) 2-Hexanone-d5	8.092	63	125444	45.300	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.600%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	72690	4.773	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	76794	5.050	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	4524	0.203	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
Data File : VV026744.D
Acq On : 13 Jul 2022 11:33
Operator : SY/MD
Sample : VV0713WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK393

Quant Time: Jul 13 23:00:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 13 23:00:17 2022
Response via : Initial Calibration

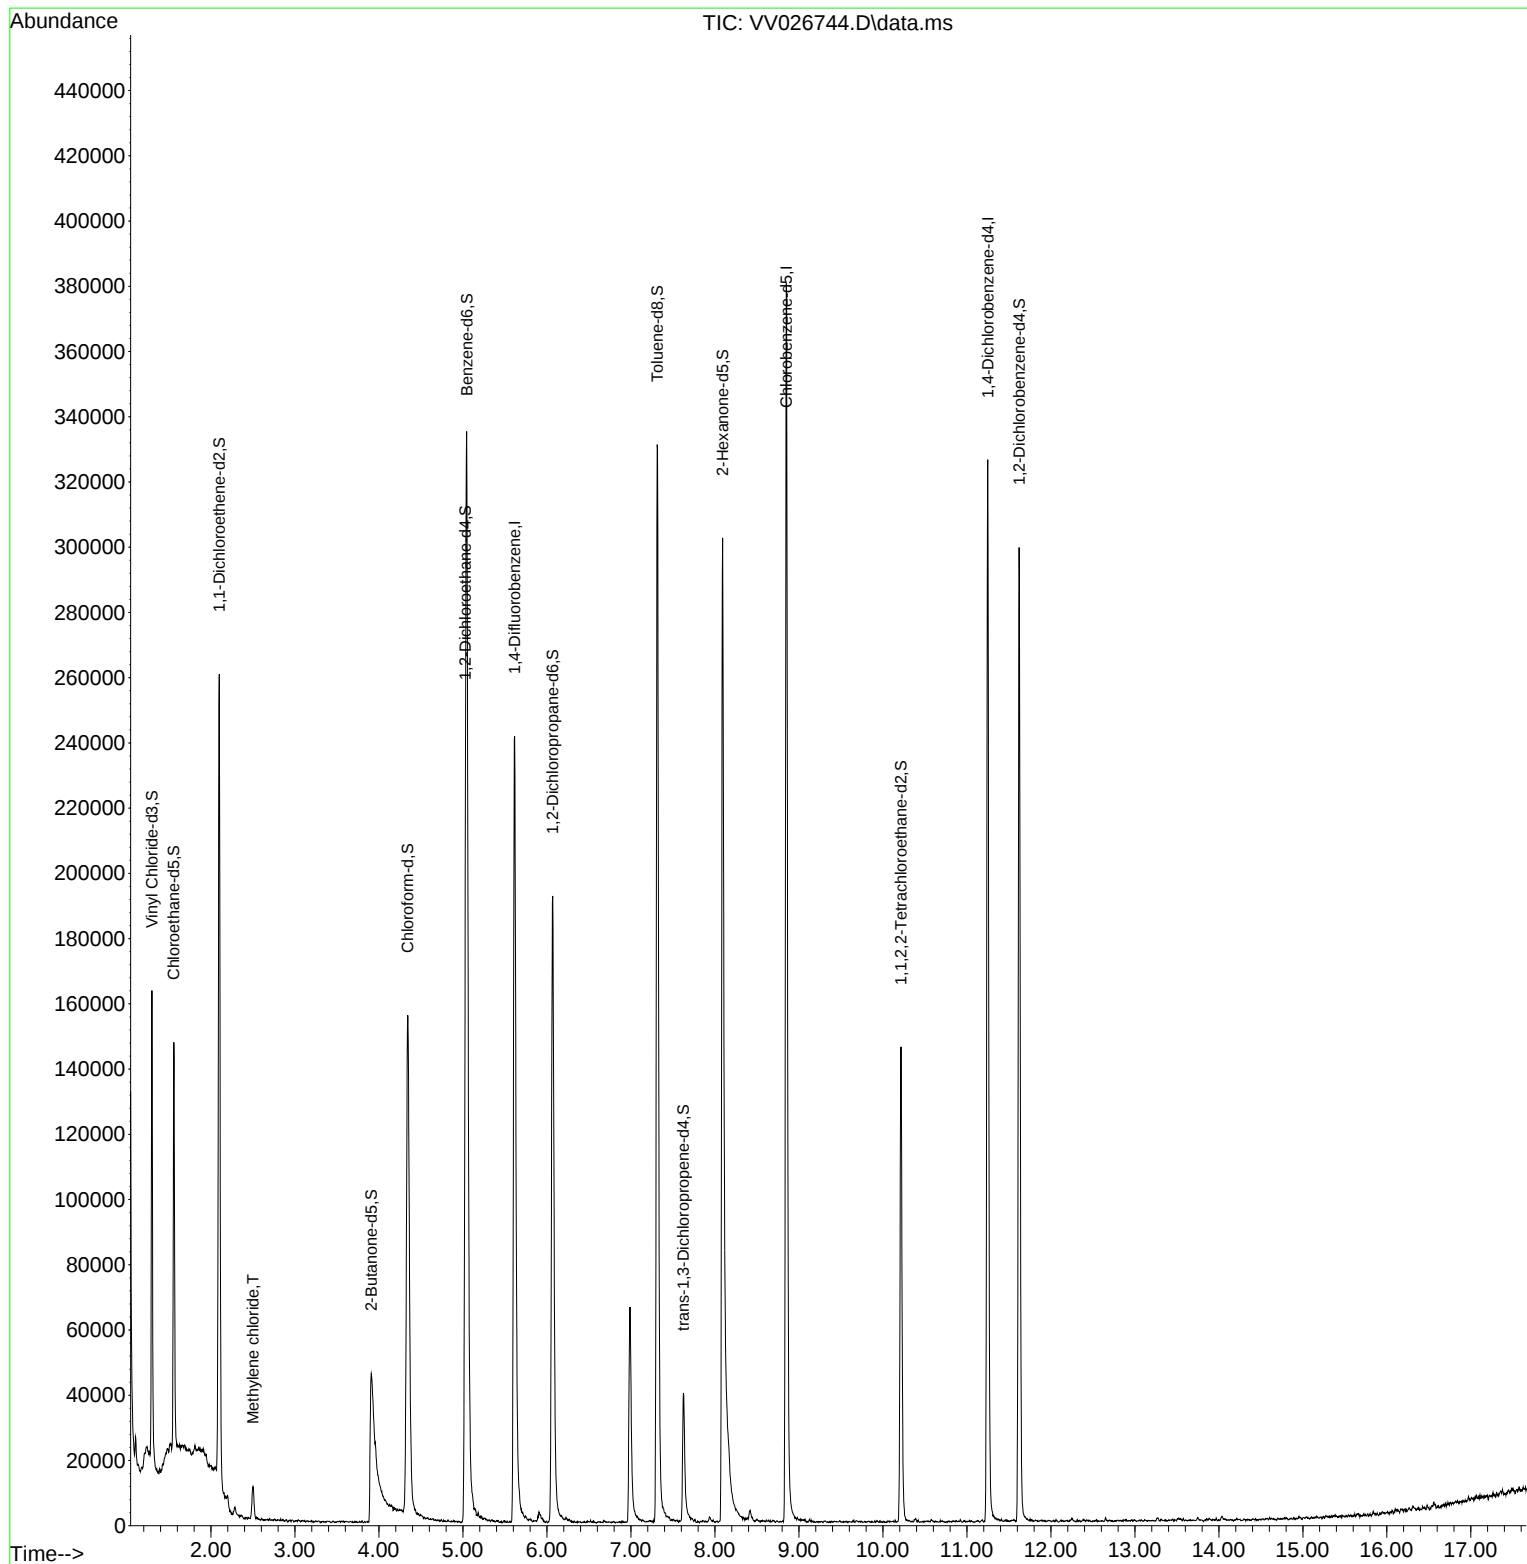

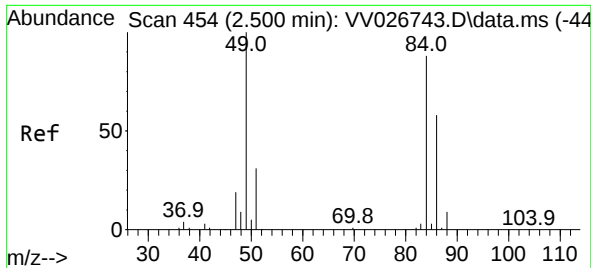

#16
Methylene chloride
Concen: 0.203 ug/L
RT: 2.500 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV026744.D
Acq: 13 Jul 2022 11:33

Instrument :
MSVOA_V
ClientSampleId :
VBLK393

Tgt Ion: 84 Resp: 4524
Ion Ratio Lower Upper
84 100
86 61.9 44.8 83.2
49 116.9 78.7 146.1

