

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071322\
 Data File : VW026745.D
 Acq On : 13 Jul 2022 11:59
 Operator : SY/MD
 Sample : N3638-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 13 23:01:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 13 23:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	236442	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.851	117	242682	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	95554	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	98415	4.563	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.200%
7) Chloroethane-d5	1.561	69	91882	4.930	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.600%
11) 1,1-Dichloroethene-d2	2.098	63	146541	3.539	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.800%
20) 2-Butanone-d5	3.912	46	148243	44.034	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.060%
24) Chloroform-d	4.346	84	189577	5.026	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.031	65	86183	5.230	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.600%
32) Benzene-d6	5.044	84	352416	4.779	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	6.066	67	111948	5.063	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.314	98	272146	4.157	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.200%
43) trans-1,3-Dichloroprop...	7.625	79	27774	3.839	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.800%
46) 2-Hexanone-d5	8.088	63	145667	46.510	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.020%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	82208	4.773	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	88690	5.327	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	12568	0.509	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
Data File : VV026745.D
Acq On : 13 Jul 2022 11:59
Operator : SY/MD
Sample : N3638-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jul 13 23:01:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 13 23:00:17 2022
Response via : Initial Calibration

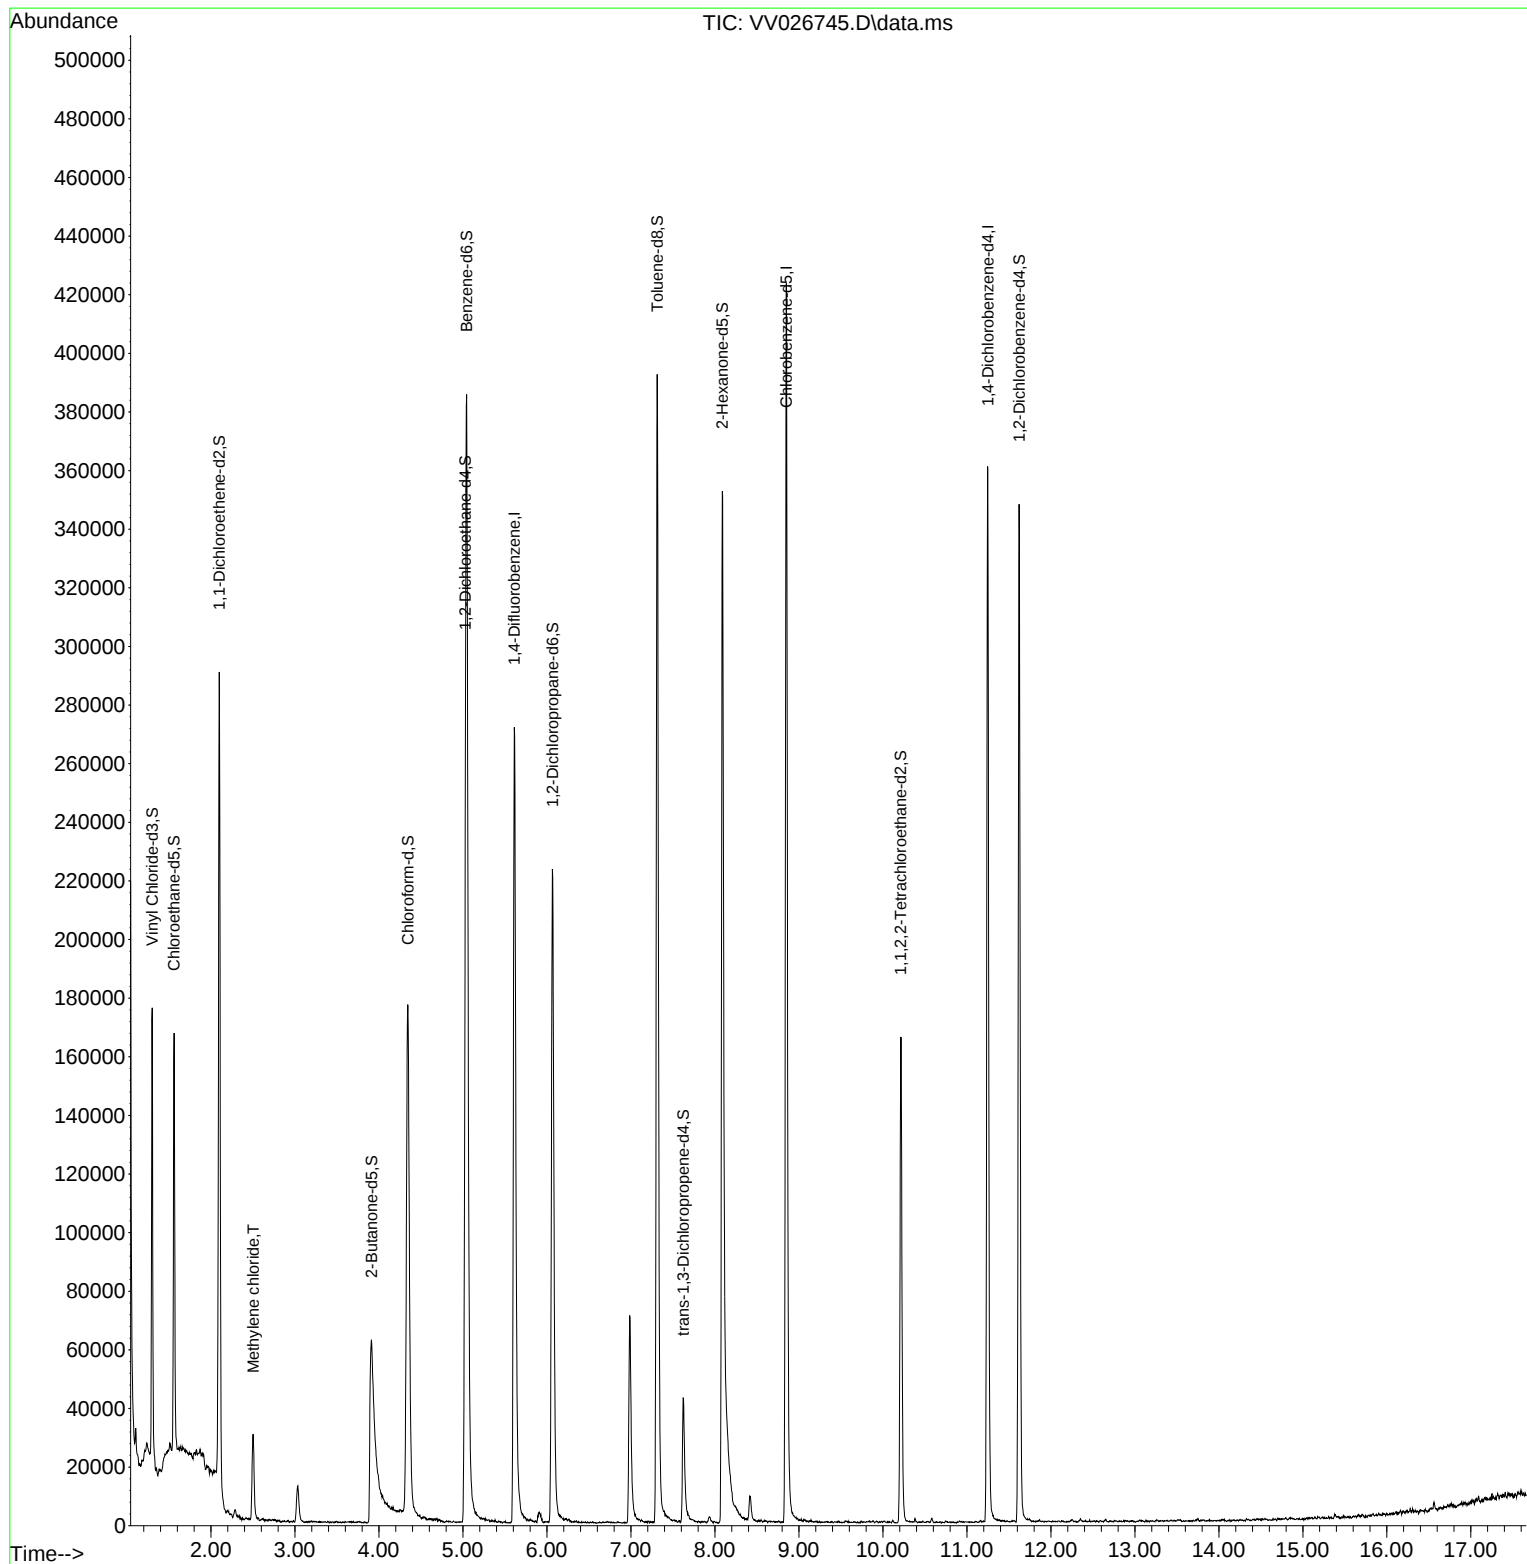

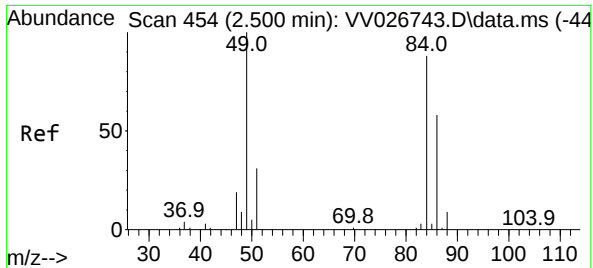

#16
Methylene chloride
Concen: 0.509 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV026745.D
Acq: 13 Jul 2022 11:59

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 12568

Ion	Ratio	Lower	Upper
84	100		
86	57.7	44.8	83.2
49	117.8	78.7	146.1

