

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
 Data File : VV026760.D
 Acq On : 13 Jul 2022 18:23
 Operator : SY/MD
 Sample : N3658-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	101	rVB	138616	151475	17.53%	2.178%
2	1.423	106	119	120	rBV2	19449	32345	3.74%	0.465%
3	1.561	155	162	171	rVB	125568	140508	16.26%	2.021%
4	2.098	320	329	349	rVB	252077	375974	43.51%	5.407%
5	2.285	377	387	398	rBV	9680	15132	1.75%	0.218%
6	2.503	444	455	467	rBV	15121	25517	2.95%	0.367%
7	3.905	880	891	931	rBV	58162	254509	29.45%	3.660%
8	4.349	1011	1029	1060	rVB3	191423	641877	74.28%	9.231%
9	5.043	1227	1245	1275	rBV2	344470	864110	100.00%	12.427%
10	5.616	1410	1423	1452	rBV	248704	520189	60.20%	7.481%
11	6.069	1547	1564	1596	rBV	199008	432905	50.10%	6.226%
12	6.985	1834	1849	1869	rBV2	68483	134453	15.56%	1.934%
13	7.313	1940	1951	1969	rBV	337456	600040	69.44%	8.630%
14	7.625	2037	2048	2070	rBV2	40025	80206	9.28%	1.154%
15	8.091	2182	2193	2233	rBV	330257	732460	84.76%	10.534%
16	8.850	2416	2429	2458	rBV	399836	658211	76.17%	9.466%
17	10.217	2842	2854	2874	rBV	156019	250726	29.02%	3.606%
18	11.249	3164	3175	3192	rBV	333375	524230	60.67%	7.539%
19	11.622	3278	3291	3310	rBV	307480	491931	56.93%	7.075%
20	16.560	4815	4827	4835	rBV3	17959	26433	3.06%	0.380%




Sum of corrected areas: 6953231

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
Data File : VV026760.D
Acq On : 13 Jul 2022 18:23
Operator : SY/MD
Sample : N3658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

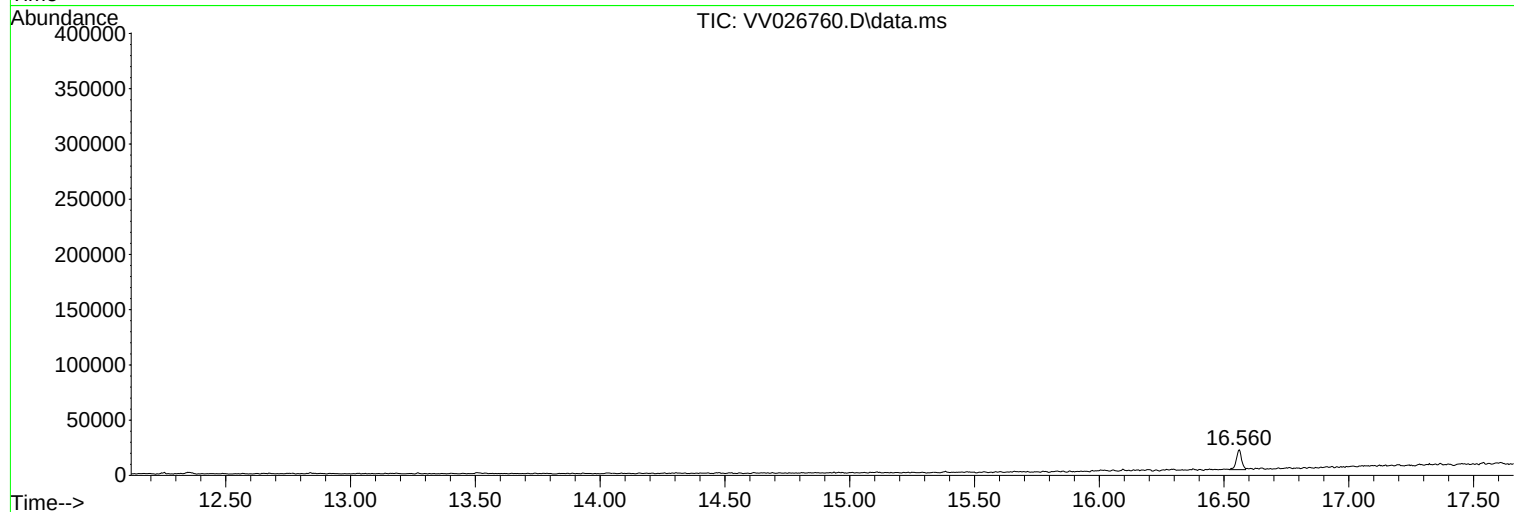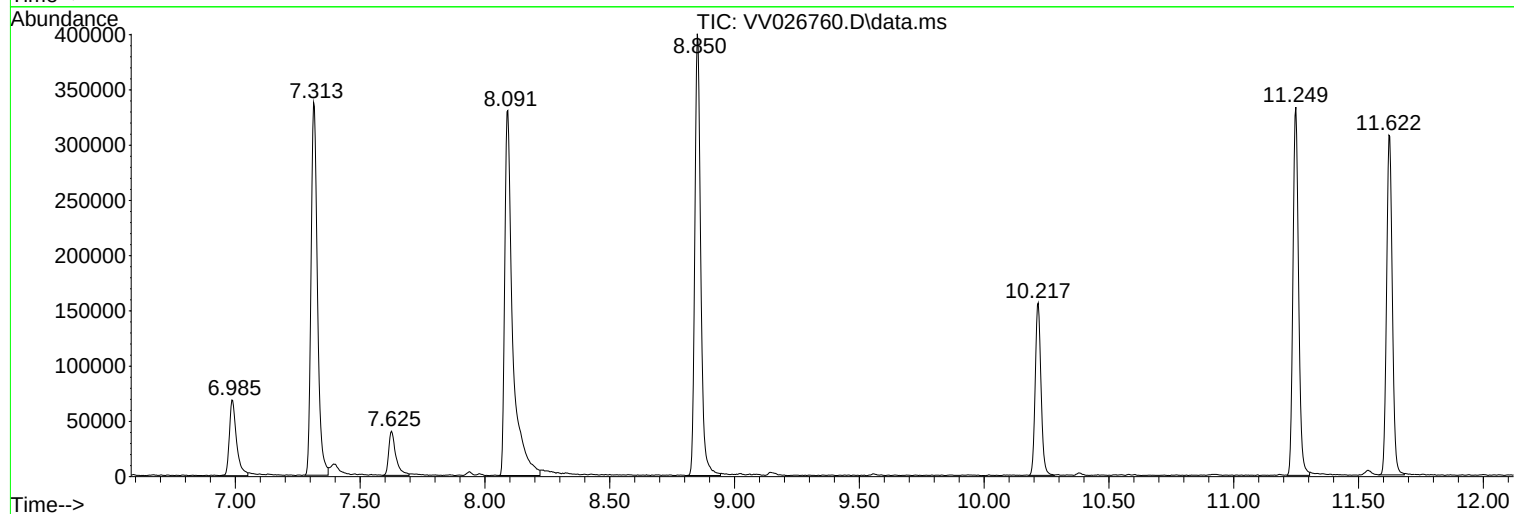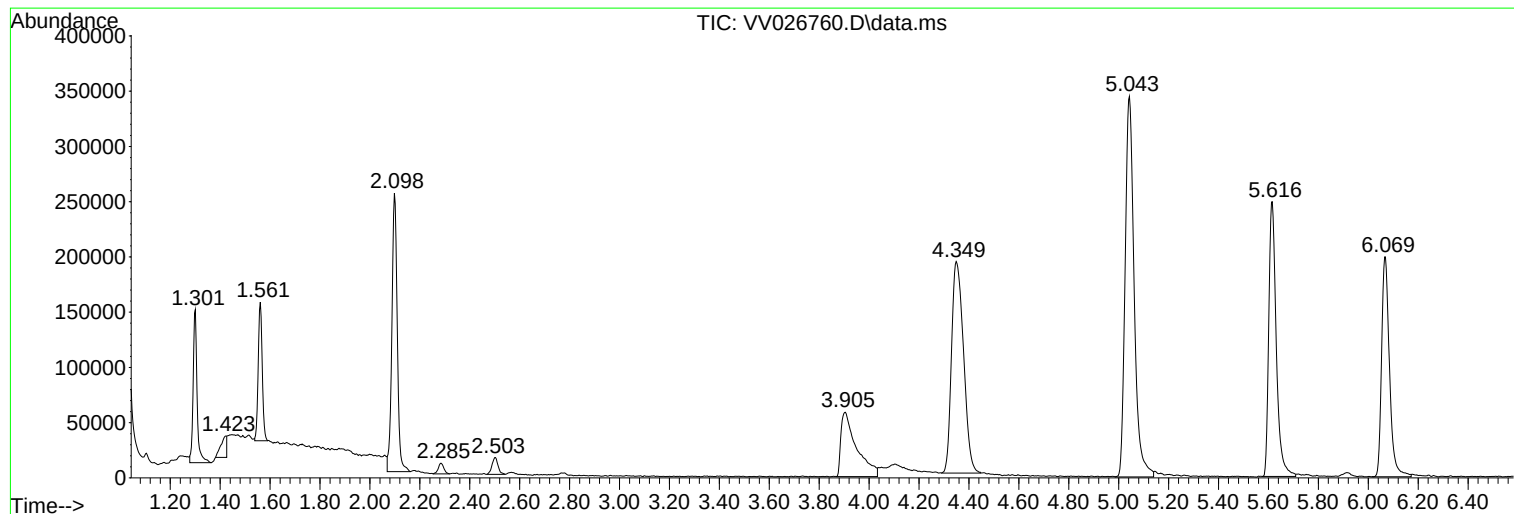

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
Data File : VV026760.D
Acq On : 13 Jul 2022 18:23
Operator : SY/MD
Sample : N3658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
Data File : VV026760.D
Acq On : 13 Jul 2022 18:23
Operator : SY/MD
Sample : N3658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------