
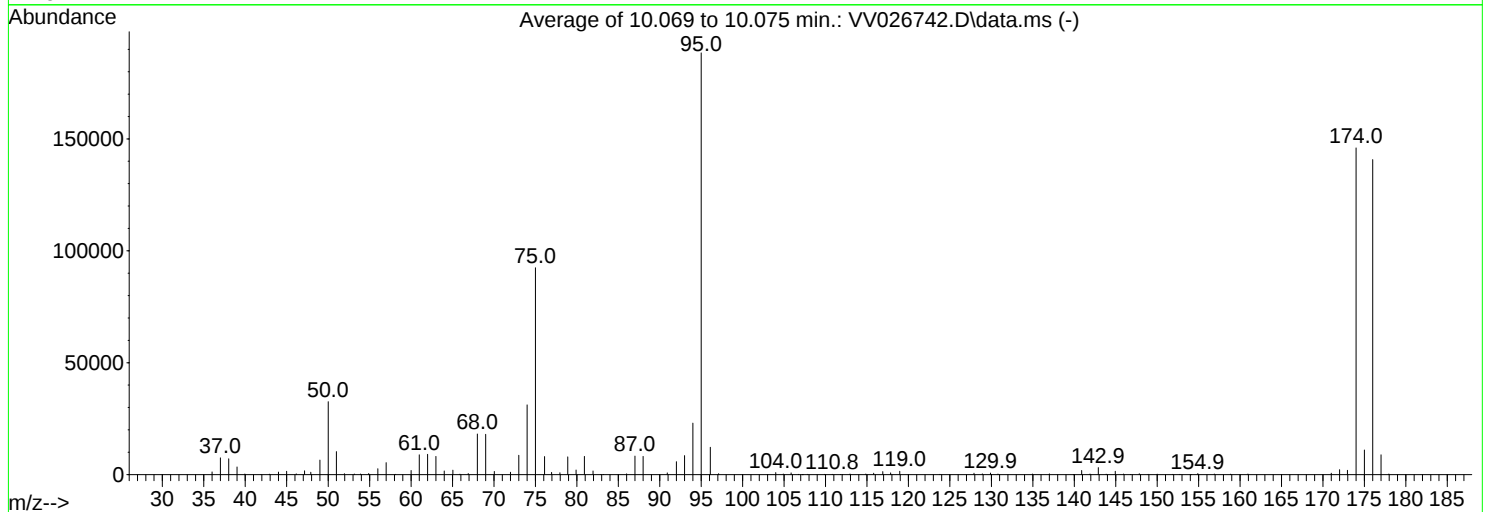


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071322\
 Data File : VV026742.D
 Acq On : 13 Jul 2022 09:23
 Operator : SY/MD
 Sample : BFB344
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB344

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jul 13 23:00:17 2022

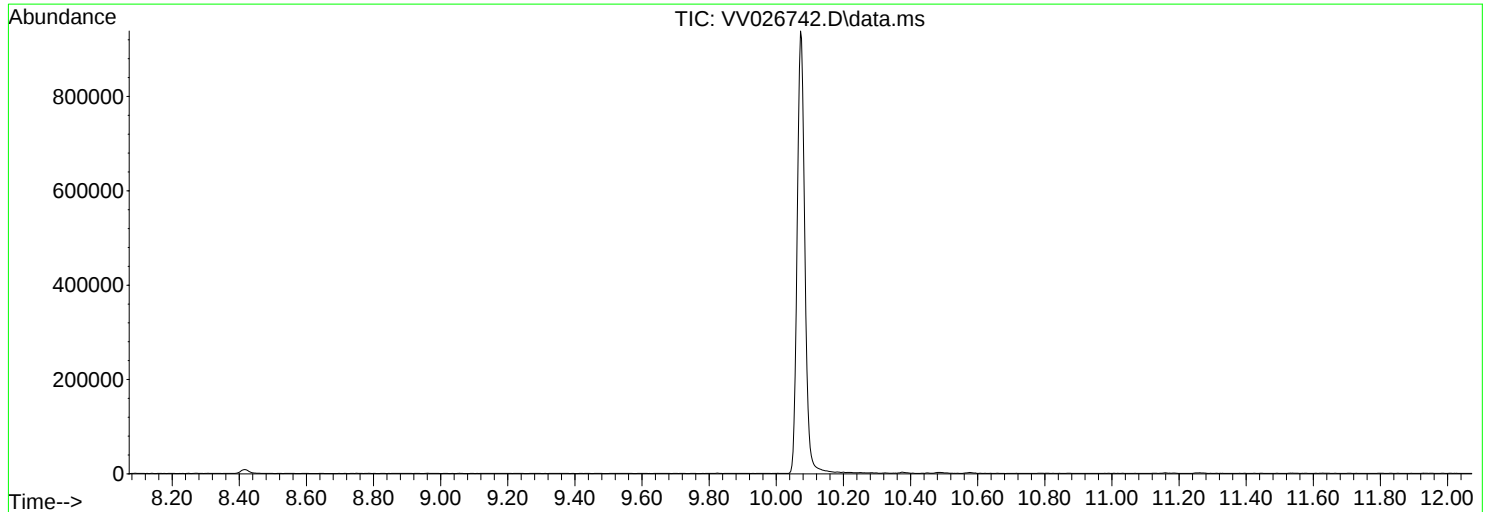

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	32605	PASS
75	95	30	80	49.1	92435	PASS
95	95	100	100	100.0	188437	PASS
96	95	5	9	6.5	12209	PASS
173	174	0.00	2	1.3	1949	PASS
174	95	50	120	77.5	145963	PASS
175	174	5	9	7.5	11010	PASS
176	174	95	105	96.4	140720	PASS
177	176	5	10	6.3	8852	PASS

m/z	Abundance
40.00	314.0
44.00	566.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344

m/z	Abundance
36.00	1228.0
37.00	7560.0
38.00	6958.0
39.00	3205.0
39.90	550.0
42.90	228.0
44.00	1773.0
45.00	1512.0
46.10	379.0
47.10	1745.0
47.90	1066.0
49.00	6338.0
50.00	32168.0
51.00	9916.0
51.90	528.0
53.10	260.0
53.90	258.0
54.90	487.0
56.00	2568.0
57.00	5291.0
58.10	183.0
60.00	1797.0
61.00	8567.0
62.00	9028.0
63.00	7539.0
64.00	1626.0
65.00	1869.0
65.90	167.0
66.90	507.0
68.00	17512.0
69.00	17536.0
70.00	1429.0
72.00	1051.0
73.00	8544.0
74.00	30456.0
75.00	88536.0
76.10	7832.0
77.00	959.0
77.90	774.0
78.90	7726.0
79.90	1967.0
80.90	7985.0
82.00	1523.0
83.00	134.0
86.00	366.0
87.00	7905.0
88.00	7504.0
90.90	723.0
92.00	5570.0
93.00	8231.0
94.00	21832.0
95.00	177792.0
96.10	11710.0
97.10	332.0
103.00	132.0
104.00	924.0
104.90	237.0
105.90	854.0
106.70	119.0
107.80	134.0
109.90	165.0
110.80	150.0
111.80	127.0
113.00	277.0
114.80	225.0
115.80	652.0
116.90	1418.0
117.80	810.0
118.90	1525.0
123.80	151.0
127.90	553.0
128.90	301.0
129.90	681.0
130.90	263.0
135.00	286.0
137.00	390.0
140.90	1808.0
141.90	281.0
142.90	2994.0
143.90	195.0
144.90	1484.0
145.90	305.0
147.80	398.0
149.00	190.0
150.00	203.0
151.90	106.0
152.80	126.0
154.90	439.0
156.90	246.0
158.90	221.0
161.00	254.0
171.00	631.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344

172.00	1876.0
173.00	1683.0
174.00	135232.0
175.00	10140.0
176.00	129872.0
177.00	8578.0
177.90	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344

m/z	Abundance
36.00	1285.0
37.00	7743.0
38.00	7314.0
39.00	3586.0
40.00	624.0
42.90	234.0
44.00	1784.0
45.00	1617.0
46.10	405.0
47.20	1849.0
47.90	1066.0
49.00	6627.0
50.00	33712.0
51.00	10819.0
51.90	458.0
53.10	304.0
53.90	259.0
54.90	554.0
56.00	2750.0
57.00	5469.0
58.10	191.0
60.00	1988.0
61.00	9226.0
62.00	9259.0
63.00	8372.0
64.00	1704.0
65.00	2075.0
65.90	221.0
66.90	523.0
68.00	18800.0
69.00	18616.0
70.10	1499.0
72.00	1104.0
73.00	8995.0
74.00	32328.0
75.00	95600.0
76.10	8359.0
76.90	1061.0
77.90	912.0
78.90	8099.0
79.90	2118.0
80.90	8364.0
81.90	1695.0
83.20	120.0
86.00	397.0
87.00	8634.0
88.00	8465.0
90.90	823.0
92.00	5969.0
93.00	8734.0
94.00	23704.0
95.00	195136.0
96.10	12655.0
97.10	430.0
103.00	116.0
104.00	1040.0
104.90	294.0
105.90	823.0
106.70	170.0
107.20	101.0
107.80	128.0
109.90	174.0
110.80	193.0
112.00	153.0
112.90	344.0
114.80	284.0
115.80	699.0
116.90	1429.0
117.80	851.0
119.00	1570.0
123.80	134.0
127.90	667.0
128.90	356.0
129.90	752.0
130.80	273.0
135.00	333.0
137.00	395.0
139.90	104.0
140.90	1925.0
141.90	264.0
142.90	3222.0
143.90	208.0
145.00	1564.0
146.00	299.0
146.80	135.0
147.80	435.0
148.90	138.0
150.00	210.0
151.90	108.0
152.70	151.0
154.90	508.0
156.90	272.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344

158.80	211.0
161.00	290.0
171.00	687.0
172.00	2311.0
173.00	1962.0
174.00	150976.0
175.00	11485.0
176.00	145728.0
177.00	9266.0
178.00	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344

m/z	Abundance
36.00	1233.0
37.00	7168.0
38.00	6912.0
39.00	3506.0
40.00	628.0
41.90	141.0
42.90	176.0
44.00	1689.0
45.00	1471.0
46.20	372.0
47.10	1670.0
47.90	995.0
49.00	6454.0
50.00	31936.0
51.00	10150.0
52.00	370.0
53.20	300.0
53.90	250.0
54.90	569.0
56.00	2689.0
57.00	5273.0
58.10	145.0
60.00	1925.0
61.00	8849.0
62.00	8978.0
63.00	8493.0
64.00	1592.0
65.10	2012.0
65.90	226.0
66.90	499.0
68.00	18096.0
69.00	17928.0
70.10	1377.0
72.00	1063.0
73.00	8471.0
74.00	30768.0
75.00	93168.0
76.10	7973.0
76.90	1020.0
78.00	933.0
78.90	7905.0
79.90	2082.0
80.90	8029.0
81.90	1750.0
82.80	103.0
83.20	110.0
86.00	360.0
87.00	8361.0
88.00	8593.0
90.90	814.0
92.00	5818.0
93.00	8610.0
94.00	23496.0
95.00	192384.0
96.10	12263.0
97.10	451.0
104.00	923.0
104.90	333.0
105.80	738.0
106.80	230.0
107.90	147.0
109.90	157.0
110.80	199.0
112.10	162.0
112.90	318.0
114.90	306.0
115.80	707.0
116.90	1306.0
117.90	809.0
119.00	1465.0
123.80	137.0
127.90	675.0
128.90	350.0
129.90	741.0
130.70	281.0
134.80	339.0
137.00	319.0
140.90	1800.0
141.90	225.0
142.90	3149.0
143.80	223.0
145.00	1480.0
146.00	305.0
146.80	174.0
147.90	495.0
148.80	124.0
150.00	211.0
151.90	127.0
152.70	130.0
154.00	105.0
154.90	535.0
156.90	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344

158.80	195.0
160.90	245.0
171.00	587.0
172.00	2375.0
172.90	2203.0
174.00	151680.0
175.00	11405.0
176.00	146560.0
177.00	8713.0
178.00	273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB344