
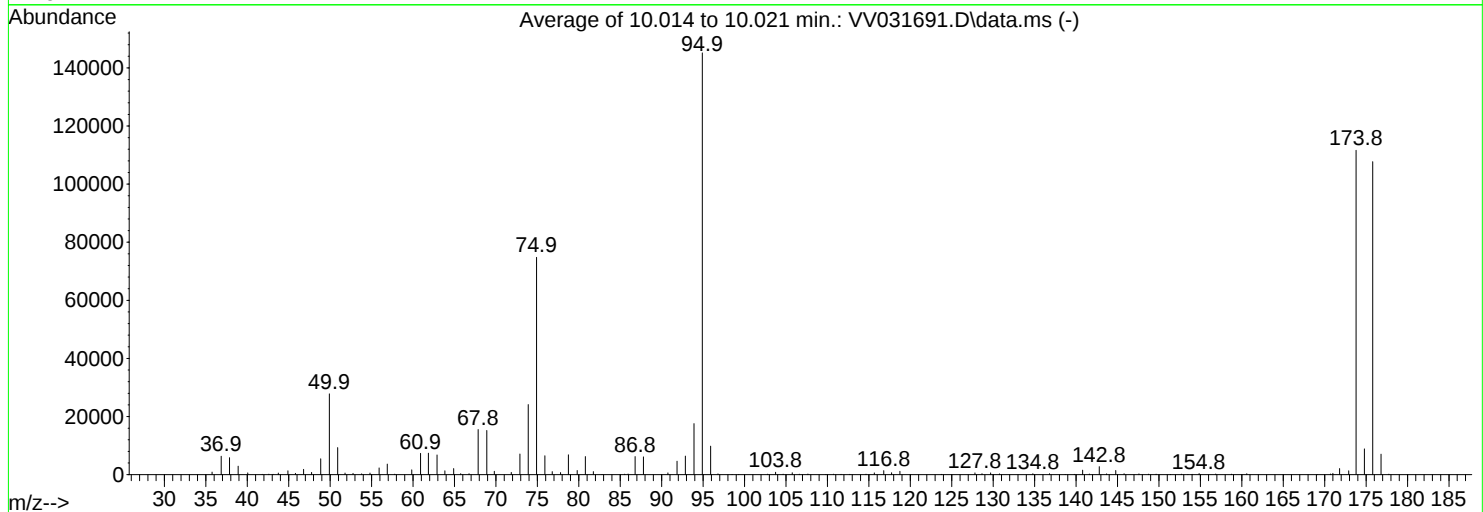


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071323\
Data File : VV031691.D
Acq On : 13 Jul 2023 11:46
Operator : SY/MD
Sample : BFB281
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB281

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jul 14 06:00:54 2023

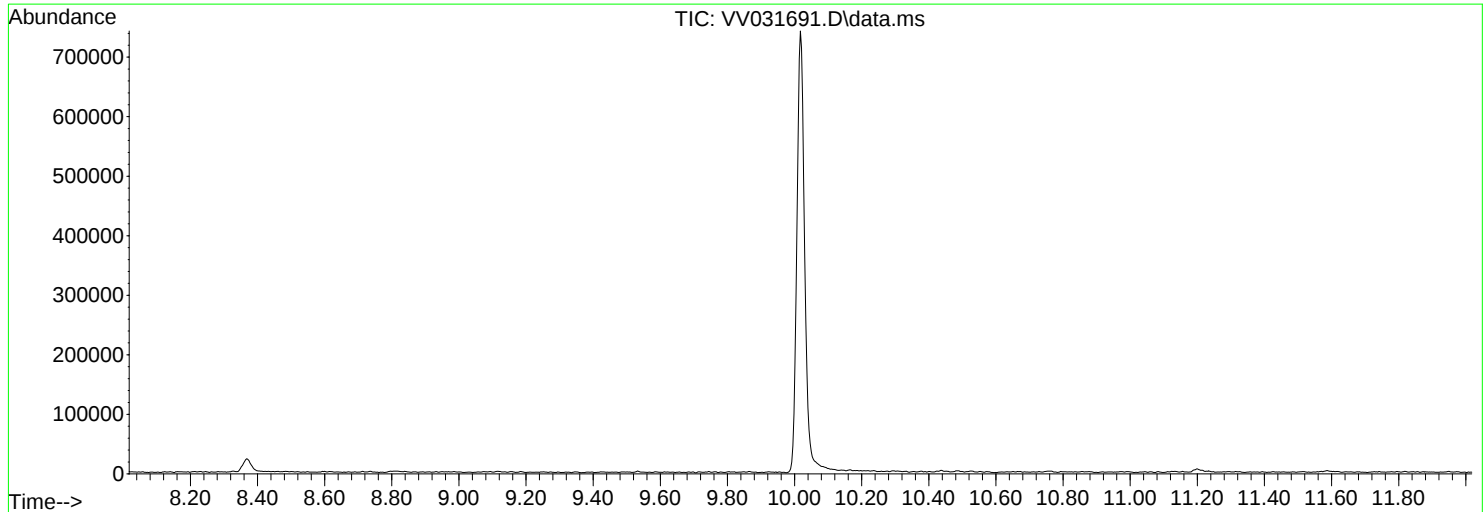

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	27827	PASS
75	95	30	80	51.5	74800	PASS
95	95	100	100	100.0	145195	PASS
96	95	5	9	6.7	9786	PASS
173	174	0.00	2	1.2	1328	PASS
174	95	50	120	76.9	111643	PASS
175	174	5	9	8.0	8891	PASS
176	174	95	105	96.5	107736	PASS
177	176	5	10	6.6	7059	PASS

m/z	Abundance
35.70	118.0
37.40	163.0
39.80	281.0
40.50	111.0
41.10	120.0
43.80	922.0
51.80	133.0
62.50	130.0
69.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
35.80	985.0
36.90	6402.0
37.90	5817.0
38.90	2814.0
40.00	687.0
41.70	148.0
42.60	163.0
43.10	144.0
43.70	1404.0
44.90	1414.0
45.80	440.0
46.80	1932.0
47.80	851.0
48.80	4979.0
49.90	27256.0
50.90	9191.0
51.80	601.0
52.70	353.0
53.80	305.0
54.80	639.0
55.90	2273.0
56.90	3704.0
57.80	204.0
59.80	1544.0
60.90	7178.0
61.90	7332.0
62.90	6671.0
63.90	1360.0
64.90	1913.0
65.70	248.0
66.80	318.0
67.90	15353.0
68.90	15022.0
69.80	1206.0
71.90	802.0
72.90	7184.0
73.90	24000.0
74.90	72144.0
75.90	6276.0
76.80	964.0
77.80	682.0
78.70	6892.0
79.80	1331.0
80.80	6242.0
81.70	1094.0
82.80	102.0
85.50	192.0
85.90	229.0
86.80	6220.0
87.80	5721.0
90.70	542.0
91.90	4386.0
92.80	6357.0
93.90	17664.0
94.90	141440.0
95.90	9568.0
96.80	280.0
98.50	106.0
99.30	123.0
102.70	142.0
103.70	837.0
104.60	239.0
105.80	745.0
106.60	166.0
107.70	172.0
110.80	118.0
111.60	141.0
112.70	107.0
114.60	154.0
115.60	539.0
116.80	1463.0
117.70	816.0
118.70	1181.0
127.80	542.0
128.60	237.0
129.70	515.0
130.80	285.0
134.80	283.0
136.80	314.0
140.80	1422.0
141.60	257.0
142.80	2934.0
143.80	202.0
144.80	1266.0
145.70	375.0
147.60	303.0
148.70	156.0
149.60	198.0
151.40	110.0
152.70	161.0
154.80	435.0
156.80	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

158.70	164.0
160.60	325.0
169.10	103.0
171.00	669.0
171.80	2125.0
172.90	1997.0
173.80	106368.0
174.80	8420.0
175.80	101632.0
176.80	6965.0
177.70	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
35.80	934.0
36.80	6597.0
37.90	6100.0
38.90	3011.0
40.10	649.0
41.80	154.0
42.60	180.0
43.10	154.0
43.80	1467.0
44.90	1371.0
45.80	432.0
46.80	1898.0
47.70	792.0
48.90	5659.0
49.90	28848.0
50.90	9625.0
51.90	679.0
52.70	434.0
53.80	304.0
54.80	552.0
55.90	2395.0
56.90	3708.0
57.70	176.0
59.90	1744.0
60.90	7562.0
61.80	7444.0
62.90	7026.0
63.80	1349.0
64.90	2138.0
65.70	368.0
66.70	337.0
67.80	16135.0
68.90	15790.0
69.80	1190.0
71.90	819.0
72.90	7329.0
73.90	24720.0
74.90	77488.0
75.90	6679.0
76.80	1108.0
77.80	708.0
78.80	6985.0
79.80	1454.0
80.80	6437.0
81.70	1098.0
85.60	197.0
85.90	213.0
86.80	6553.0
87.80	6302.0
90.80	584.0
91.90	4827.0
92.90	6644.0
93.90	18128.0
94.90	150464.0
95.90	10177.0
96.80	282.0
99.30	126.0
102.80	162.0
103.80	834.0
104.60	194.0
105.70	711.0
106.60	184.0
107.60	207.0
110.80	164.0
111.60	125.0
112.70	137.0
114.70	164.0
115.60	628.0
116.80	1445.0
117.70	720.0
118.80	1195.0
123.80	133.0
127.80	641.0
128.70	332.0
129.70	642.0
130.80	291.0
134.80	334.0
136.80	368.0
138.70	105.0
139.80	139.0
140.80	1574.0
141.60	260.0
142.80	2815.0
143.70	279.0
144.80	1503.0
145.80	325.0
147.60	281.0
148.70	158.0
149.70	202.0
152.70	137.0
153.50	104.0
154.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

154.80	427.0
156.90	241.0
158.80	154.0
160.60	366.0
171.00	667.0
171.80	2141.0
172.90	1986.0
173.80	115608.0
174.80	9164.0
175.80	111432.0
176.80	7349.0
177.80	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
35.80	1009.0
36.80	6071.0
37.80	5580.0
38.90	2891.0
40.00	550.0
41.90	117.0
42.60	146.0
43.80	1552.0
44.90	1188.0
45.80	388.0
46.80	1691.0
47.80	760.0
48.80	5797.0
49.90	27376.0
50.90	9057.0
51.90	722.0
52.80	490.0
53.80	315.0
54.80	422.0
55.90	2338.0
56.90	3449.0
57.90	165.0
59.90	1735.0
60.90	7181.0
61.80	7354.0
62.90	6681.0
63.80	1305.0
64.90	2187.0
65.80	375.0
66.70	335.0
67.80	15209.0
68.90	15397.0
69.80	1072.0
71.80	729.0
72.90	6822.0
73.90	23688.0
74.90	74768.0
75.90	6520.0
76.80	1083.0
77.80	721.0
78.80	6669.0
79.80	1466.0
80.80	5938.0
81.80	1040.0
85.60	192.0
86.00	224.0
86.80	5988.0
87.80	6307.0
90.80	627.0
91.80	4720.0
92.90	6257.0
93.90	16936.0
94.90	143680.0
95.90	9612.0
96.80	233.0
102.90	154.0
103.80	809.0
104.70	161.0
105.70	624.0
106.60	135.0
107.70	226.0
109.80	108.0
110.70	208.0
111.70	123.0
112.70	162.0
114.70	121.0
115.70	673.0
116.80	1261.0
117.80	527.0
118.80	1169.0
123.70	174.0
127.80	670.0
128.70	422.0
129.70	662.0
130.70	270.0
134.80	387.0
136.80	310.0
139.80	185.0
140.80	1581.0
141.60	235.0
142.80	2599.0
143.60	411.0
144.80	1550.0
145.90	281.0
147.60	258.0
148.80	144.0
149.70	192.0
152.70	143.0
154.00	188.0
154.90	328.0
156.90	235.0
158.80	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

160.60	270.0
170.70	683.0
171.80	2061.0
173.80	112952.0
174.80	9089.0
175.80	110144.0
176.80	6864.0
177.80	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281