


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071420\
 Data File : VV017471.D
 Acq On : 14 Jul 2020 08:53
 Operator : SY/MD
 Sample : BFB49
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 15 02:49:58 2020

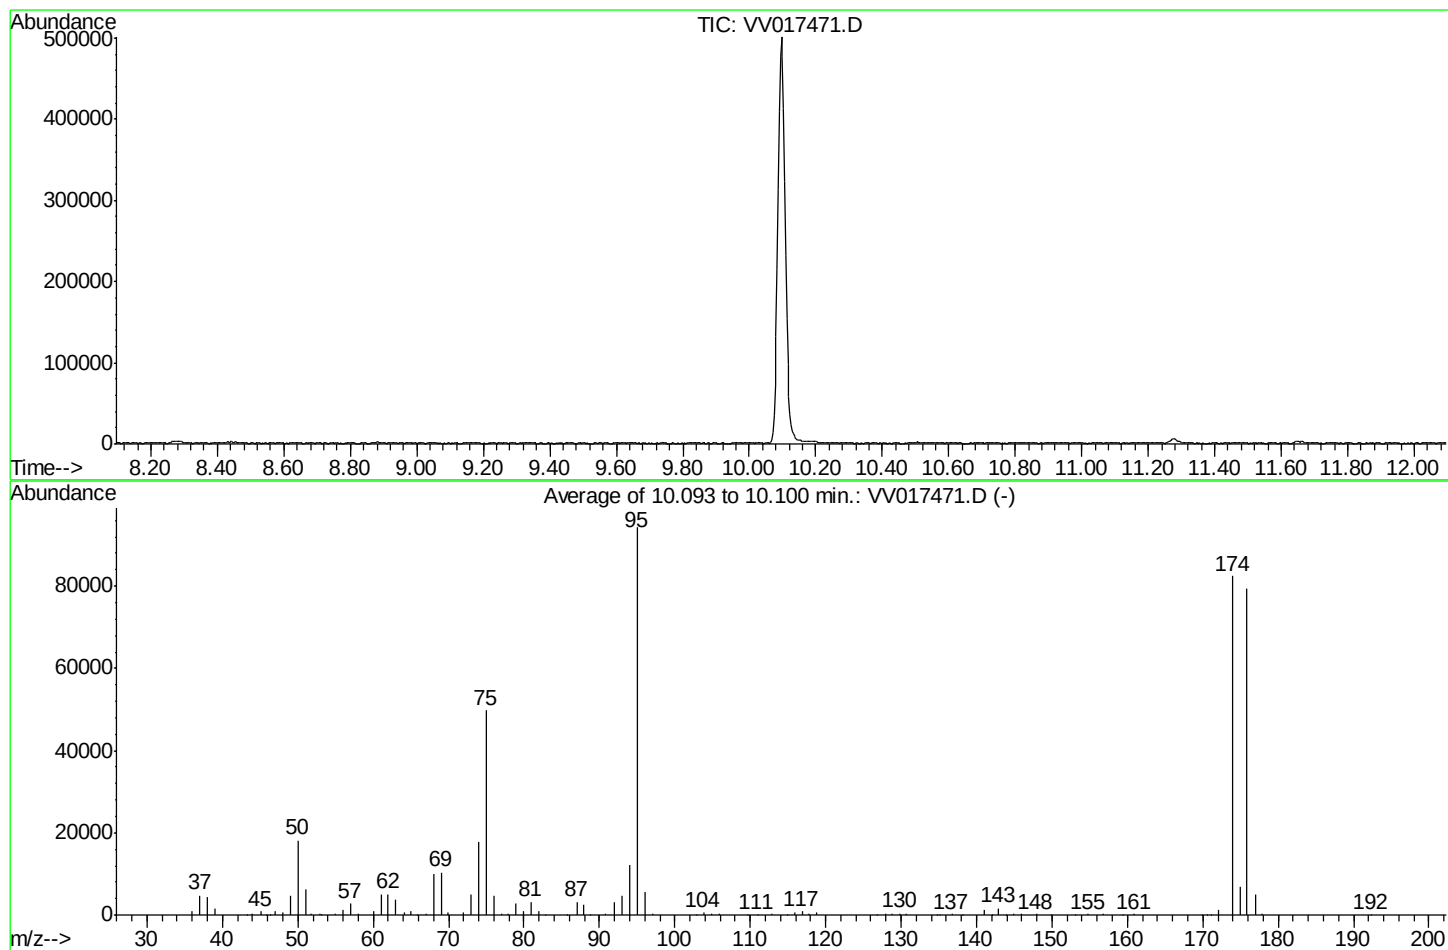

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	18202	PASS
75	95	30	80	52.7	49722	PASS
95	95	100	100	100.0	94330	PASS
96	95	5	9	6.0	5682	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.4	82416	PASS
175	174	5	9	8.4	6896	PASS
176	174	95	101	96.5	79504	PASS
177	176	5	9	6.1	4861	PASS

m/z	Abundance
36.00	991.0
37.00	4729.0
38.00	4307.0
39.00	1920.0
39.90	230.0
44.00	789.0
45.00	729.0
46.20	150.0
47.00	756.0
47.90	739.0
49.00	4402.0
50.00	18256.0
51.00	6014.0
51.90	371.0
52.90	188.0
55.00	350.0
56.00	1374.0
57.00	2702.0
58.10	133.0
60.00	955.0
61.00	4853.0
62.00	5428.0
63.00	3936.0
64.10	535.0
65.00	907.0
65.90	142.0
67.00	343.0
68.00	9883.0
69.00	9753.0
70.00	559.0
72.00	707.0
73.00	4978.0
74.00	17208.0
75.00	49696.0
76.00	4820.0
77.00	475.0
78.00	285.0
79.00	2795.0
79.90	1118.0
80.90	3264.0
81.90	754.0
82.80	155.0
85.70	141.0
87.00	3166.0
87.90	2357.0
88.80	129.0
90.90	463.0
92.00	2809.0
92.90	4407.0
94.00	11846.0
95.00	93416.0
96.00	5951.0
97.20	200.0
103.80	510.0
104.90	200.0
105.90	395.0
109.60	110.0
110.90	107.0
112.80	254.0
115.80	503.0
116.90	858.0
117.80	418.0
118.90	611.0
127.90	348.0
128.80	257.0
129.80	363.0
130.70	251.0
134.70	109.0
135.00	124.0
136.80	248.0
141.00	1159.0
142.90	1436.0
144.00	153.0
145.00	252.0
146.00	194.0
148.00	314.0
149.90	132.0
154.80	259.0
156.80	225.0
160.90	222.0
169.80	125.0
171.00	241.0
172.00	1160.0
174.00	79744.0
175.00	6981.0
175.90	76504.0
177.00	4733.0
177.90	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	1050.0
37.00	4827.0
38.00	4566.0
39.00	1881.0
40.00	223.0
44.00	785.0
45.00	836.0
46.30	159.0
47.00	833.0
47.90	715.0
49.00	4889.0
50.00	18808.0
51.00	6392.0
51.90	348.0
52.80	183.0
55.00	305.0
56.00	1365.0
57.00	2776.0
58.10	194.0
60.00	1093.0
61.00	5248.0
62.00	5268.0
63.00	3842.0
64.00	496.0
65.00	850.0
65.90	142.0
67.00	416.0
68.00	10043.0
69.00	10749.0
69.90	553.0
72.00	651.0
73.00	5393.0
74.00	18216.0
75.00	51032.0
76.00	4825.0
76.90	434.0
77.90	275.0
78.90	2841.0
79.90	1058.0
80.90	3346.0
81.90	822.0
82.80	151.0
85.70	109.0
87.00	3264.0
88.00	2457.0
88.80	121.0
90.80	438.0
92.00	3089.0
93.00	4612.0
94.00	12869.0
95.00	97360.0
96.00	5795.0
97.00	172.0
97.20	181.0
102.80	107.0
103.80	549.0
104.90	189.0
105.90	446.0
110.90	128.0
112.80	230.0
115.80	519.0
116.90	887.0
117.80	490.0
118.90	629.0
126.80	119.0
127.90	387.0
128.80	288.0
129.80	371.0
130.60	227.0
134.80	155.0
136.80	290.0
140.90	1160.0
142.90	1700.0
143.90	141.0
145.00	343.0
146.00	176.0
148.00	268.0
149.90	157.0
153.10	102.0
154.80	301.0
156.80	267.0
161.00	208.0
169.80	116.0
172.00	1127.0
174.00	85272.0
175.00	7113.0
175.90	82320.0
177.00	4878.0
177.90	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	956.0
37.00	4516.0
38.00	4262.0
39.00	1707.0
40.00	220.0
43.20	103.0
44.00	781.0
45.10	875.0
45.80	118.0
46.30	134.0
47.00	787.0
48.00	652.0
49.00	4550.0
50.00	17544.0
51.00	5892.0
51.90	248.0
52.80	168.0
53.10	148.0
55.00	255.0
56.00	1310.0
57.00	2708.0
58.00	229.0
60.00	1077.0
61.00	5087.0
62.00	4728.0
63.00	3575.0
64.00	412.0
65.00	707.0
65.90	123.0
67.00	421.0
68.00	9563.0
69.00	10548.0
69.90	502.0
72.00	506.0
73.00	4878.0
74.00	17480.0
75.00	48440.0
76.00	4215.0
76.90	423.0
78.90	2707.0
79.90	954.0
80.90	3122.0
81.90	823.0
82.90	127.0
87.00	2958.0
88.00	2371.0
90.80	399.0
91.90	3164.0
93.00	4569.0
94.00	12174.0
95.00	92216.0
96.00	5300.0
97.00	175.0
103.90	448.0
104.80	170.0
105.90	418.0
110.90	130.0
112.80	173.0
114.80	108.0
115.90	471.0
116.90	796.0
117.80	487.0
118.80	650.0
126.70	134.0
127.90	346.0
128.90	290.0
129.90	358.0
130.60	190.0
134.80	214.0
136.70	322.0
138.10	101.0
140.90	1179.0
142.10	180.0
142.90	1828.0
143.80	146.0
145.00	386.0
146.00	170.0
147.90	206.0
149.90	147.0
154.80	328.0
156.90	246.0
159.40	117.0
161.00	187.0
170.50	133.0
172.00	1030.0
174.00	82232.0
175.00	6595.0
175.90	79688.0
177.00	4973.0
177.90	171.0
192.30	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	115.0
38.80	132.0
39.90	240.0
44.00	334.0
51.70	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49