

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021648.D
 Acq On : 14 Jul 2021 10:37
 Operator : SY/MD
 Sample : VV0714MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	229634	223768	13.58%	1.747%
2	1.558	155	161	180	rVB	171014	201245	12.21%	1.571%
3	2.105	321	331	356	rVB	356847	531030	32.22%	4.146%
4	2.503	448	455	467	rVB2	7978	13134	0.80%	0.103%
5	2.609	486	488	491	rBV2	436	222	0.01%	0.002%
6	2.802	545	548	555	rBV2	566	383	0.02%	0.003%
7	3.053	623	626	628	rBV	321	207	0.01%	0.002%
8	3.111	640	644	645	rBV2	426	267	0.02%	0.002%
9	3.281	694	697	699	rBV2	318	161	0.01%	0.001%
10	3.381	727	728	731	rVB	289	116	0.01%	0.001%
11	3.413	735	738	740	rBV	408	257	0.02%	0.002%
12	3.461	751	753	757	rVB2	370	223	0.01%	0.002%
13	3.529	770	774	779	rVB2	371	290	0.02%	0.002%
14	3.571	785	787	791	rVB2	421	212	0.01%	0.002%
15	3.683	818	822	826	rBV4	399	440	0.03%	0.003%
16	3.761	845	846	853	rBV3	213	211	0.01%	0.002%
17	3.867	870	879	927	rVV	139207	367656	22.31%	2.871%
18	4.204	981	984	988	rBV2	651	488	0.03%	0.004%
19	4.346	1011	1028	1054	rBV2	257132	639605	38.81%	4.994%
20	4.596	1104	1106	1111	rBV2	704	464	0.03%	0.004%
21	4.850	1182	1185	1186	rBV	358	227	0.01%	0.002%
22	4.876	1191	1193	1196	rVB3	361	176	0.01%	0.001%
23	4.905	1198	1202	1208	rBV4	384	354	0.02%	0.003%
24	4.937	1210	1212	1216	rBV3	383	291	0.02%	0.002%
25	4.979	1222	1225	1226	rBV2	281	142	0.01%	0.001%
26	5.043	1226	1245	1280	rBV2	645040	1648161	100.00%	12.869%
27	5.362	1342	1344	1348	rVB3	697	325	0.02%	0.003%
28	5.384	1348	1351	1356	rBV3	729	578	0.04%	0.005%
29	5.506	1387	1389	1392	rVB3	797	405	0.02%	0.003%
30	5.526	1392	1395	1398	rBV3	371	257	0.02%	0.002%
31	5.551	1398	1403	1407	rBV3	453	404	0.02%	0.003%
32	5.613	1409	1422	1453	rBV	508555	1031750	62.60%	8.056%
33	5.905	1504	1513	1533	rVB2	17302	37666	2.29%	0.294%
34	6.014	1544	1547	1549	rBV2	239	140	0.01%	0.001%
35	6.069	1550	1564	1588	rBV	357563	737950	44.77%	5.762%
36	6.375	1657	1659	1661	rVB2	314	136	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021648.D
 Acq On : 14 Jul 2021 10:37
 Operator : SY/MD
 Sample : VV0714MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.487	1692	1694	1695	rBV2	300	109	0.01%	0.001%
38	6.500	1695	1698	1699	rBV	408	211	0.01%	0.002%
39	6.593	1725	1727	1729	rBV2	251	155	0.01%	0.001%
40	6.625	1734	1737	1738	rBV	520	246	0.01%	0.002%
41	6.677	1747	1753	1758	rBV4	648	835	0.05%	0.007%
42	6.741	1770	1773	1775	rBV3	203	136	0.01%	0.001%
43	6.760	1777	1779	1781	rVB	287	128	0.01%	0.001%
44	6.873	1812	1814	1817	rVB	321	167	0.01%	0.001%
45	6.915	1824	1827	1829	rBV2	190	127	0.01%	0.001%
46	6.944	1833	1836	1837	rBV	314	137	0.01%	0.001%
47	6.985	1837	1849	1879	rBV	221500	402564	24.43%	3.143%
48	7.313	1938	1951	1970	rBV	790150	1373157	83.31%	10.722%
49	7.584	2032	2035	2036	rBV2	439	226	0.01%	0.002%
50	7.622	2036	2047	2074	rVV	149481	262493	15.93%	2.050%
51	7.866	2121	2123	2124	rBV	438	206	0.01%	0.002%
52	7.950	2146	2149	2152	rVV2	409	247	0.01%	0.002%
53	7.979	2157	2158	2160	rBV	600	273	0.02%	0.002%
54	8.034	2172	2175	2177	rBV	399	199	0.01%	0.002%
55	8.043	2177	2178	2180	rBV	323	169	0.01%	0.001%
56	8.085	2181	2191	2226	rBV	422026	792379	48.08%	6.187%
57	8.506	2320	2322	2324	rBV	279	108	0.01%	0.001%
58	8.609	2353	2354	2358	rVB	557	371	0.02%	0.003%
59	8.638	2358	2363	2364	rBV2	262	201	0.01%	0.002%
60	8.673	2371	2374	2379	rVB3	403	372	0.02%	0.003%
61	8.702	2379	2383	2387	rBV2	394	355	0.02%	0.003%
62	8.754	2396	2399	2401	rBV3	205	173	0.01%	0.001%
63	8.854	2417	2430	2460	rBV	749434	1228950	74.56%	9.596%
64	9.063	2493	2495	2497	rVB	507	236	0.01%	0.002%
65	9.127	2512	2515	2519	rBV2	643	627	0.04%	0.005%
66	9.300	2566	2569	2571	rBV	294	168	0.01%	0.001%
67	9.397	2597	2599	2603	rBV2	573	376	0.02%	0.003%
68	9.464	2618	2620	2624	rBV2	224	166	0.01%	0.001%
69	9.493	2627	2629	2631	rBV	260	116	0.01%	0.001%
70	9.548	2642	2646	2652	rBV5	949	1222	0.07%	0.010%
71	9.593	2655	2660	2662	rVB3	632	474	0.03%	0.004%
72	9.680	2685	2687	2694	rVB3	600	555	0.03%	0.004%
73	9.709	2694	2696	2698	rBV2	236	155	0.01%	0.001%
74	9.850	2738	2740	2742	rVB2	437	196	0.01%	0.002%
75	10.069	2804	2808	2813	rVB3	281	287	0.02%	0.002%
76	10.098	2814	2817	2818	rBV	353	185	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021648.D
 Acq On : 14 Jul 2021 10:37
 Operator : SY/MD
 Sample : VV0714MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	10.127	2818	2826	2839	rVB2	5289	7504	0.46%	0.059%
78	10.217	2841	2854	2882	rBV	495932	788149	47.82%	6.154%
79	10.413	2912	2915	2918	rVB3	558	343	0.02%	0.003%
80	10.429	2918	2920	2924	rVB	296	184	0.01%	0.001%
81	10.464	2928	2931	2933	rBV	390	214	0.01%	0.002%
82	10.545	2950	2956	2959	rBV4	1169	1449	0.09%	0.011%
83	10.661	2988	2992	2994	rBV2	403	348	0.02%	0.003%
84	10.747	3017	3019	3023	rVB	468	243	0.01%	0.002%
85	10.770	3024	3026	3028	rBV2	400	181	0.01%	0.001%
86	10.895	3062	3065	3066	rBV3	787	439	0.03%	0.003%
87	10.921	3066	3073	3082	rVB5	5194	7636	0.46%	0.060%
88	11.001	3095	3098	3101	rBV	240	177	0.01%	0.001%
89	11.146	3137	3143	3151	rVB4	2280	3266	0.20%	0.026%
90	11.249	3164	3175	3197	rBV	800360	1234422	74.90%	9.639%
91	11.500	3250	3253	3255	rBV	569	343	0.02%	0.003%
92	11.542	3263	3266	3268	rBV2	470	269	0.02%	0.002%
93	11.625	3280	3292	3313	rBV	776751	1233956	74.87%	9.635%
94	11.841	3355	3359	3360	rBV2	1062	746	0.05%	0.006%
95	11.924	3379	3385	3390	rBV2	474	551	0.03%	0.004%
96	12.249	3481	3486	3488	rBV3	873	769	0.05%	0.006%
97	12.599	3592	3595	3596	rBV2	558	292	0.02%	0.002%
98	12.648	3607	3610	3612	rBV3	1630	1260	0.08%	0.010%
99	13.268	3799	3803	3816	rVB6	3300	4790	0.29%	0.037%
100	13.513	3871	3879	3888	rBV3	6739	10857	0.66%	0.085%




Sum of corrected areas: 12807186

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021648.D
Acq On : 14 Jul 2021 10:37
Operator : SY/MD
Sample : VV0714MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

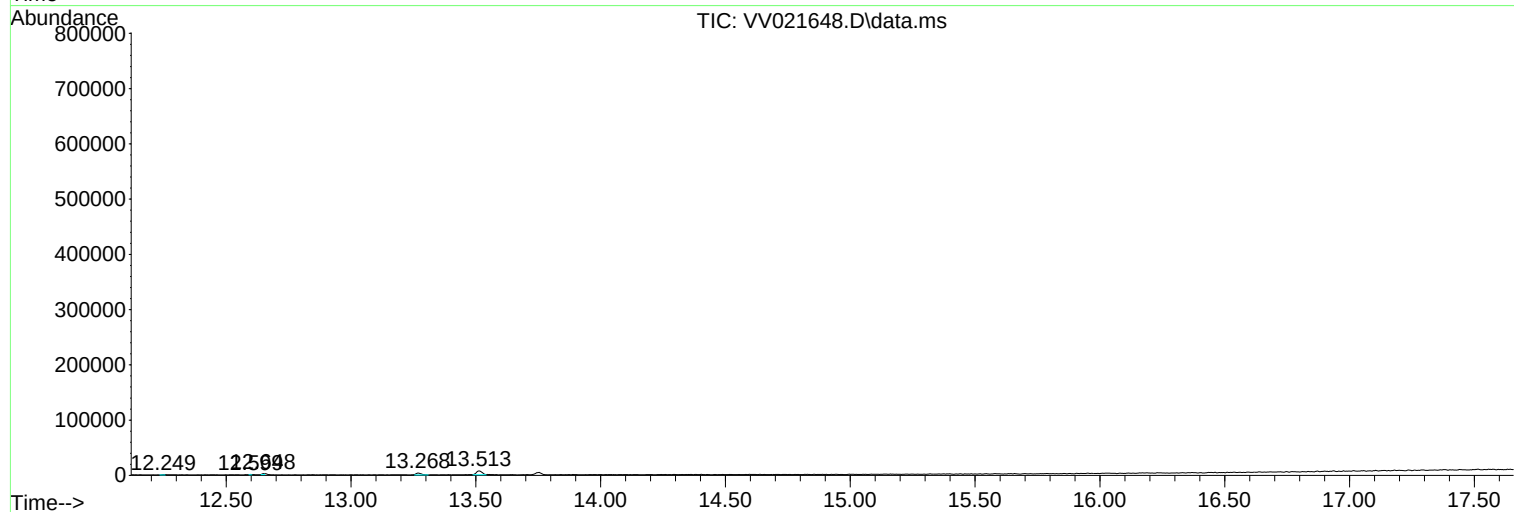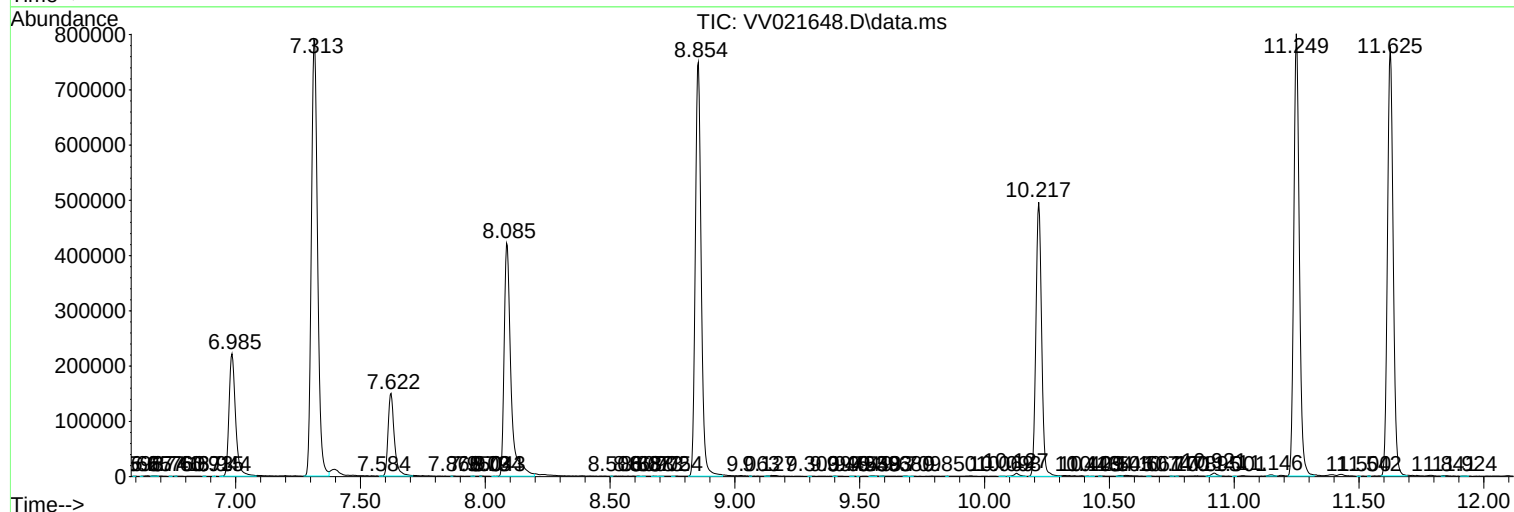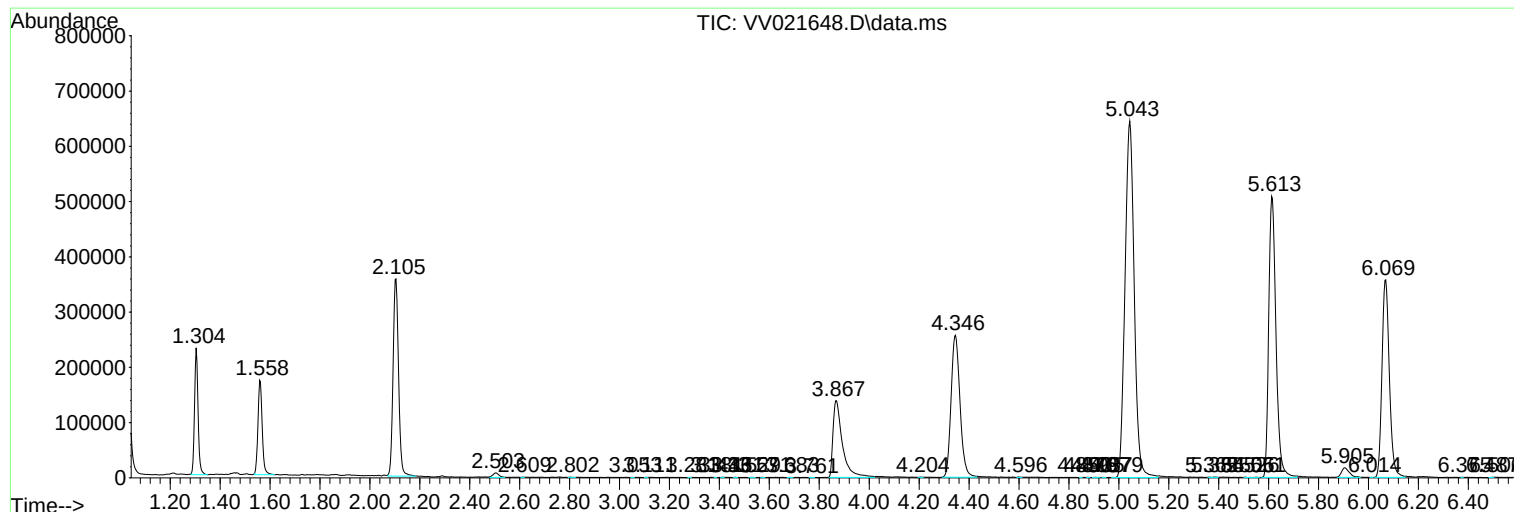

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021648.D
Acq On : 14 Jul 2021 10:37
Operator : SY/MD
Sample : VV0714MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021648.D
Acq On : 14 Jul 2021 10:37
Operator : SY/MD
Sample : VV0714MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
