

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021657.D
 Acq On : 14 Jul 2021 16:48
 Operator : SY/MD
 Sample : M3033-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	45	49	59	rVB2	35277	35539	2.29%	0.280%
2	1.304	75	82	92	rBV	198647	194178	12.50%	1.531%
3	1.558	154	161	182	rVB	156736	184809	11.90%	1.457%
4	2.101	321	330	350	rVB	318014	469883	30.24%	3.704%
5	2.503	448	455	465	rVB2	5379	9033	0.58%	0.071%
6	2.613	485	489	492	rBV3	1035	1053	0.07%	0.008%
7	2.690	510	513	517	rVB2	367	258	0.02%	0.002%
8	2.767	521	537	562	rBV2	245153	513798	33.07%	4.050%
9	2.940	589	591	594	rBV2	385	235	0.02%	0.002%
10	2.979	601	603	604	rBV	417	193	0.01%	0.002%
11	3.040	612	622	633	rBV5	2029	4284	0.28%	0.034%
12	3.098	638	640	643	rVB3	358	180	0.01%	0.001%
13	3.114	643	645	648	rBV2	283	165	0.01%	0.001%
14	3.281	690	697	701	rBV3	822	978	0.06%	0.008%
15	3.346	715	717	720	rVB	410	146	0.01%	0.001%
16	3.365	720	723	726	rBV3	347	248	0.02%	0.002%
17	3.394	729	732	734	rVV2	233	162	0.01%	0.001%
18	3.403	734	735	740	rVB2	355	155	0.01%	0.001%
19	3.497	762	764	766	rBV2	321	190	0.01%	0.001%
20	3.513	766	769	775	rVB2	591	460	0.03%	0.004%
21	3.551	779	781	784	rVB2	241	142	0.01%	0.001%
22	3.600	793	796	800	rBV	282	230	0.01%	0.002%
23	3.625	800	804	806	rVB2	319	212	0.01%	0.002%
24	3.664	813	816	820	rBV2	284	226	0.01%	0.002%
25	3.741	836	840	841	rBV2	561	394	0.03%	0.003%
26	3.873	870	881	920	rBV	143715	378694	24.38%	2.985%
27	4.349	1012	1029	1056	rBV	245982	604316	38.90%	4.764%
28	4.834	1177	1180	1181	rBV	397	237	0.02%	0.002%
29	4.883	1192	1195	1200	rBV2	327	187	0.01%	0.001%
30	4.947	1211	1215	1219	rBV2	411	325	0.02%	0.003%
31	4.973	1219	1223	1228	rVB4	423	437	0.03%	0.003%
32	5.047	1228	1246	1273	rBV2	612676	1553615	100.00%	12.248%
33	5.519	1389	1393	1396	rBV2	416	374	0.02%	0.003%
34	5.555	1400	1404	1406	rBV	529	367	0.02%	0.003%
35	5.616	1411	1423	1451	rBV	491709	985211	63.41%	7.767%
36	5.908	1504	1514	1531	rBV2	17697	36144	2.33%	0.285%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071421\
 Data File : VW021657.D
 Acq On : 14 Jul 2021 16:48
 Operator : SY/MD
 Sample : M3033-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.001	1541	1543	1549	rVB2	547	390	0.03%	0.003%
38	6.072	1549	1565	1592	rBV	342377	702796	45.24%	5.540%
39	6.255	1620	1622	1626	rBV3	752	439	0.03%	0.003%
40	6.294	1632	1634	1637	rVB3	545	238	0.02%	0.002%
41	6.313	1637	1640	1643	rVB3	503	268	0.02%	0.002%
42	6.336	1643	1647	1650	rVB3	316	221	0.01%	0.002%
43	6.352	1650	1652	1655	rVB	343	177	0.01%	0.001%
44	6.371	1655	1658	1660	rBV2	650	385	0.02%	0.003%
45	6.403	1665	1668	1673	rBV3	490	334	0.02%	0.003%
46	6.503	1697	1699	1700	rBV2	402	168	0.01%	0.001%
47	6.612	1731	1733	1735	rBV2	256	156	0.01%	0.001%
48	6.632	1737	1739	1740	rBV	550	295	0.02%	0.002%
49	6.702	1759	1761	1762	rBV2	462	201	0.01%	0.002%
50	6.770	1778	1782	1785	rVB2	326	174	0.01%	0.001%
51	6.792	1786	1789	1794	rBV2	409	320	0.02%	0.003%
52	6.870	1809	1813	1815	rVB	238	146	0.01%	0.001%
53	6.902	1820	1823	1826	rBV2	421	268	0.02%	0.002%
54	6.989	1835	1850	1877	rBV	207768	379186	24.41%	2.989%
55	7.317	1940	1952	1971	rBV	734779	1280925	82.45%	10.098%
56	7.622	2037	2047	2069	rBV	140715	242804	15.63%	1.914%
57	7.905	2132	2135	2140	rVB2	425	386	0.02%	0.003%
58	7.937	2143	2145	2150	rBV2	244	202	0.01%	0.002%
59	7.976	2154	2157	2158	rBV2	540	248	0.02%	0.002%
60	8.050	2176	2180	2182	rVB	243	159	0.01%	0.001%
61	8.088	2182	2192	2235	rBV	447748	825841	53.16%	6.510%
62	8.384	2282	2284	2286	rBV2	447	208	0.01%	0.002%
63	8.400	2286	2289	2293	rVB3	899	585	0.04%	0.005%
64	8.439	2297	2301	2305	rBV4	378	366	0.02%	0.003%
65	8.500	2317	2320	2325	rVB4	376	285	0.02%	0.002%
66	8.603	2349	2352	2353	rBV	424	262	0.02%	0.002%
67	8.625	2357	2359	2364	rVV3	507	362	0.02%	0.003%
68	8.661	2367	2370	2375	rVV2	471	445	0.03%	0.004%
69	8.689	2378	2379	2383	rVV	541	230	0.01%	0.002%
70	8.715	2385	2387	2393	rVB3	342	257	0.02%	0.002%
71	8.796	2410	2412	2415	rBV	396	249	0.02%	0.002%
72	8.853	2418	2430	2460	rBV	723938	1180301	75.97%	9.305%
73	9.111	2508	2510	2516	rBV4	405	310	0.02%	0.002%
74	9.152	2516	2523	2528	rBV5	1575	1972	0.13%	0.016%
75	9.529	2636	2640	2642	rVB3	530	363	0.02%	0.003%
76	9.548	2642	2646	2648	rBV2	755	618	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021657.D
 Acq On : 14 Jul 2021 16:48
 Operator : SY/MD
 Sample : M3033-08 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

77	9.603	2661	2663	2665	rBV	444	249	0.02%	0.002%
78	9.683	2683	2688	2690	rVB3	253	210	0.01%	0.002%
79	9.786	2717	2720	2722	rBV	319	214	0.01%	0.002%
80	9.866	2742	2745	2750	rVB3	417	343	0.02%	0.003%
81	9.934	2764	2766	2773	rVB3	460	364	0.02%	0.003%
82	9.988	2780	2783	2787	rBV	289	211	0.01%	0.002%
83	10.127	2819	2826	2836	rVB5	2937	4594	0.30%	0.036%
84	10.217	2842	2854	2879	rBV	482054	762905	49.11%	6.014%
85	10.448	2923	2926	2927	rBV	430	227	0.01%	0.002%
86	10.548	2949	2957	2959	rBV5	878	975	0.06%	0.008%
87	10.857	3050	3053	3055	rBV2	845	513	0.03%	0.004%
88	11.024	3103	3105	3106	rBV	518	200	0.01%	0.002%
89	11.146	3134	3143	3150	rBV4	2299	3367	0.22%	0.027%
90	11.181	3152	3154	3156	rBV	361	196	0.01%	0.002%
91	11.252	3164	3176	3194	rBV	747375	1158563	74.57%	9.133%
92	11.625	3281	3292	3314	rBV	726270	1147615	73.87%	9.047%
93	11.786	3337	3342	3348	rBV6	1210	1730	0.11%	0.014%
94	11.956	3391	3395	3396	rBV	195	146	0.01%	0.001%
95	12.239	3480	3483	3484	rBV2	438	240	0.02%	0.002%
96	12.734	3635	3637	3639	rVB	395	143	0.01%	0.001%
97	12.805	3656	3659	3663	rVB4	517	418	0.03%	0.003%
98	12.892	3684	3686	3689	rVB2	472	246	0.02%	0.002%
99	13.416	3846	3849	3850	rBV	353	220	0.01%	0.002%
100	13.828	3974	3977	3980	rBV3	635	454	0.03%	0.004%




Sum of corrected areas: 12684941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021657.D
Acq On : 14 Jul 2021 16:48
Operator : SY/MD
Sample : M3033-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

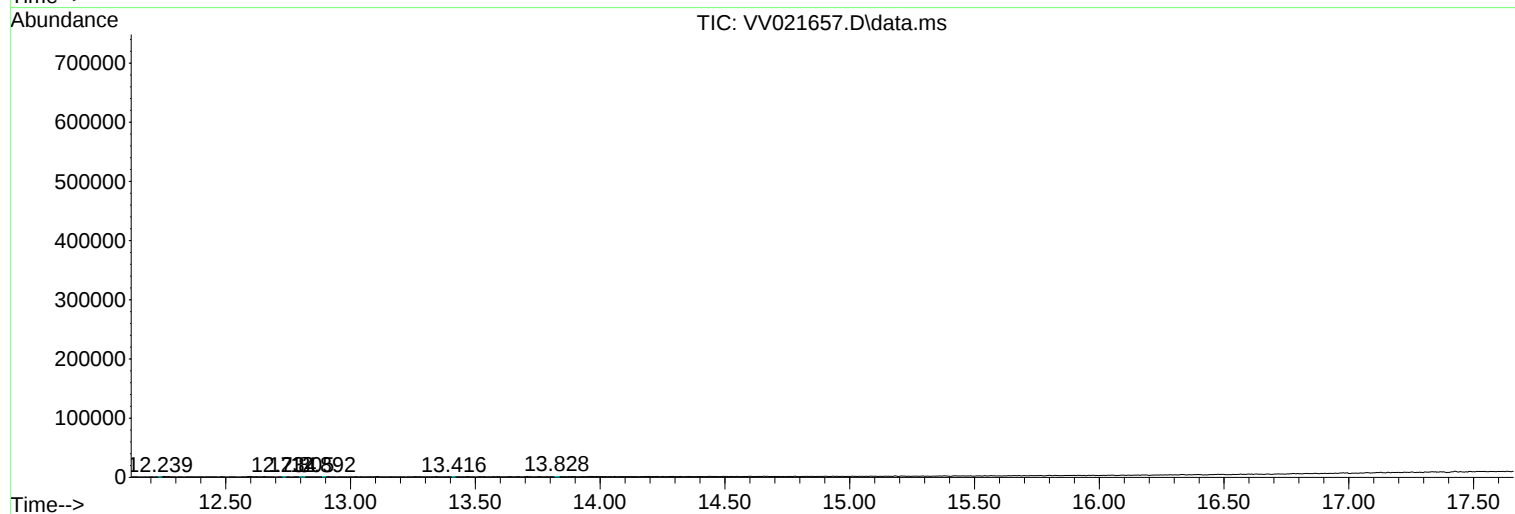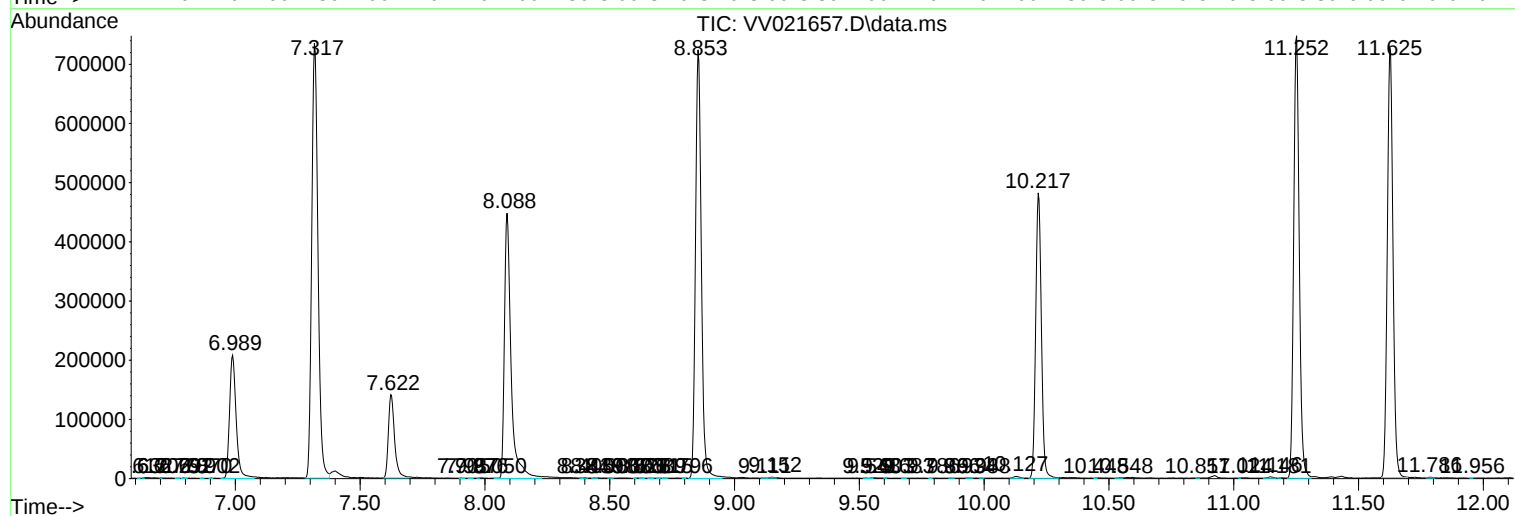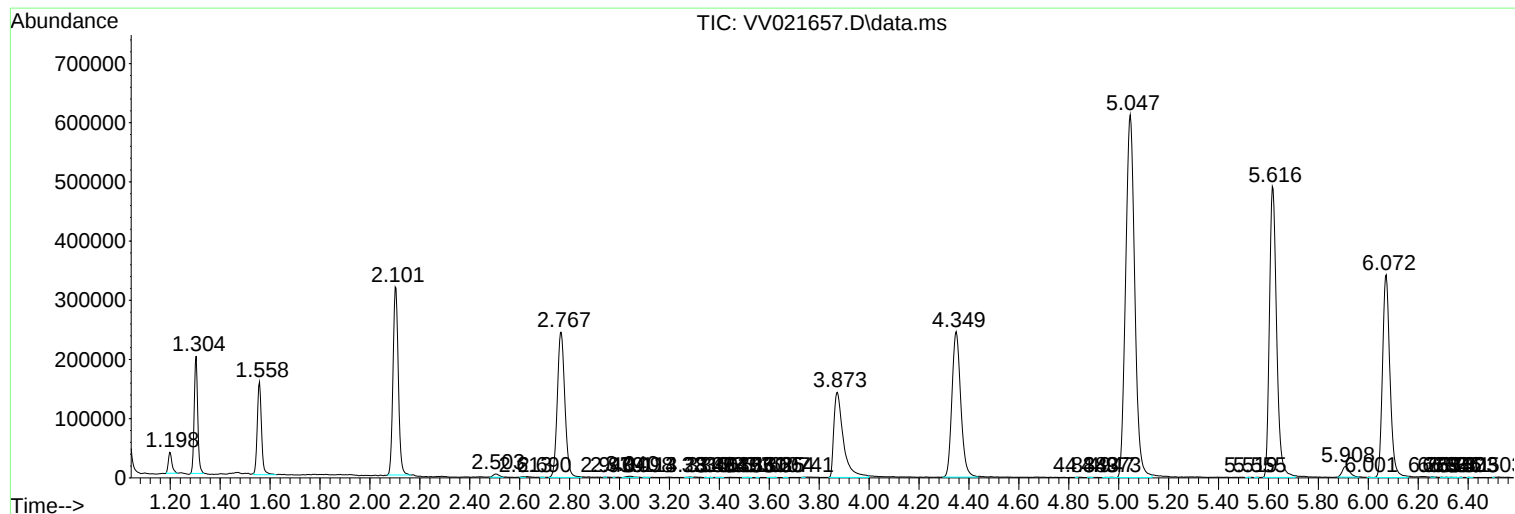

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021657.D
Acq On : 14 Jul 2021 16:48
Operator : SY/MD
Sample : M3033-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021657.D
Acq On : 14 Jul 2021 16:48
Operator : SY/MD
Sample : M3033-08 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
