

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021658.D
 Acq On : 14 Jul 2021 17:12
 Operator : SY/MD
 Sample : M3033-09 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	62	rVB	48071	47928	3.02%	0.383%
2	1.304	76	82	96	rVB	198771	199899	12.59%	1.599%
3	1.558	154	161	177	rVB	157699	182056	11.47%	1.456%
4	2.105	322	331	345	rBV	329670	475982	29.98%	3.808%
5	2.905	576	580	583	rBV2	478	408	0.03%	0.003%
6	2.979	601	603	606	rVB	415	182	0.01%	0.001%
7	3.140	652	653	654	rBV	306	110	0.01%	0.001%
8	3.198	668	671	675	rBV	261	214	0.01%	0.002%
9	3.268	690	693	695	rBV2	537	368	0.02%	0.003%
10	3.455	746	751	753	rBV2	236	215	0.01%	0.002%
11	3.468	753	755	758	rVB	288	131	0.01%	0.001%
12	3.487	759	761	763	rBV	224	119	0.01%	0.001%
13	3.522	769	772	773	rBV	237	118	0.01%	0.001%
14	3.567	783	786	789	rBV3	201	151	0.01%	0.001%
15	3.667	813	817	818	rBV2	288	208	0.01%	0.002%
16	3.725	832	835	836	rBV	230	145	0.01%	0.001%
17	3.818	862	864	867	rVB	298	153	0.01%	0.001%
18	3.873	871	881	929	rBV	154709	429023	27.03%	3.432%
19	4.349	1012	1029	1056	rBV	249547	619415	39.02%	4.955%
20	4.667	1125	1128	1129	rBV	290	133	0.01%	0.001%
21	4.815	1172	1174	1176	rBV2	167	98	0.01%	0.001%
22	4.838	1176	1181	1185	rVB3	243	256	0.02%	0.002%
23	4.857	1185	1187	1190	rVB	204	82	0.01%	0.001%
24	4.873	1190	1192	1193	rBV	178	79	0.00%	0.001%
25	4.911	1202	1204	1207	rBV2	328	198	0.01%	0.002%
26	4.924	1207	1208	1211	rVB2	849	260	0.02%	0.002%
27	4.944	1212	1214	1218	rVB2	549	277	0.02%	0.002%
28	4.973	1218	1223	1225	rBV2	527	430	0.03%	0.003%
29	5.047	1229	1246	1274	rBV2	622813	1587483	100.00%	12.699%
30	5.400	1353	1356	1357	rBV	462	281	0.02%	0.002%
31	5.452	1370	1372	1374	rBV	430	221	0.01%	0.002%
32	5.619	1411	1424	1455	rBV	502867	1008857	63.55%	8.071%
33	5.911	1503	1515	1535	rBV2	18593	39145	2.47%	0.313%
34	6.072	1551	1565	1592	rBV	349152	719886	45.35%	5.759%
35	6.294	1631	1634	1635	rBV2	519	250	0.02%	0.002%
36	6.329	1642	1645	1646	rBV2	438	257	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021658.D
 Acq On : 14 Jul 2021 17:12
 Operator : SY/MD
 Sample : M3033-09 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	6.374	1656	1659	1663	rVB2	420	238	0.01%	0.002%
38	6.391	1663	1664	1667	rBV2	256	127	0.01%	0.001%
39	6.429	1672	1676	1680	rVB2	407	339	0.02%	0.003%
40	6.452	1680	1683	1684	rBV	162	78	0.00%	0.001%
41	6.506	1698	1700	1702	rBV2	258	172	0.01%	0.001%
42	6.683	1754	1755	1758	rBV2	366	227	0.01%	0.002%
43	6.776	1783	1784	1787	rVB	290	115	0.01%	0.001%
44	6.796	1789	1790	1791	rBV	279	102	0.01%	0.001%
45	6.831	1798	1801	1803	rVB2	410	272	0.02%	0.002%
46	6.844	1803	1805	1809	rBV2	347	242	0.02%	0.002%
47	6.927	1827	1831	1833	rVB	474	282	0.02%	0.002%
48	6.944	1833	1836	1838	rVB	226	94	0.01%	0.001%
49	6.989	1838	1850	1878	rBV	211119	385865	24.31%	3.087%
50	7.317	1940	1952	1971	rBV	752325	1302961	82.08%	10.423%
51	7.622	2038	2047	2072	rBV	140351	249159	15.70%	1.993%
52	7.889	2128	2130	2132	rBV	367	202	0.01%	0.002%
53	7.937	2140	2145	2148	rBV3	646	610	0.04%	0.005%
54	7.953	2148	2150	2155	rVB2	395	262	0.02%	0.002%
55	8.088	2181	2192	2229	rBV	455297	850096	53.55%	6.801%
56	8.407	2288	2291	2293	rBV2	542	323	0.02%	0.003%
57	8.519	2323	2326	2329	rBV3	312	250	0.02%	0.002%
58	8.558	2336	2338	2340	rBV2	344	153	0.01%	0.001%
59	8.625	2358	2359	2361	rBV	263	99	0.01%	0.001%
60	8.638	2361	2363	2364	rBV	251	118	0.01%	0.001%
61	8.725	2389	2390	2394	rBV2	282	201	0.01%	0.002%
62	8.757	2397	2400	2402	rVB2	661	367	0.02%	0.003%
63	8.773	2402	2405	2411	rBV3	650	586	0.04%	0.005%
64	8.805	2411	2415	2418	rBV2	290	271	0.02%	0.002%
65	8.853	2418	2430	2456	rBV	734397	1209546	76.19%	9.676%
66	9.114	2507	2511	2513	rBV3	454	321	0.02%	0.003%
67	9.140	2517	2519	2520	rBV2	820	322	0.02%	0.003%
68	9.230	2542	2547	2549	rBV2	491	336	0.02%	0.003%
69	9.242	2549	2551	2557	rVB4	200	139	0.01%	0.001%
70	9.268	2557	2559	2560	rBV4	306	134	0.01%	0.001%
71	9.336	2578	2580	2582	rBV	256	119	0.01%	0.001%
72	9.406	2599	2602	2605	rBV2	338	268	0.02%	0.002%
73	9.497	2624	2630	2632	rBV2	389	322	0.02%	0.003%
74	9.532	2638	2641	2644	rVB2	188	115	0.01%	0.001%
75	9.554	2644	2648	2651	rBV3	651	560	0.04%	0.004%
76	9.570	2651	2653	2655	rVB	274	112	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
 Data File : VV021658.D
 Acq On : 14 Jul 2021 17:12
 Operator : SY/MD
 Sample : M3033-09 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7M7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.622	2664	2669	2670	rBV	227	153	0.01%	0.001%
78	9.706	2693	2695	2698	rVB2	201	100	0.01%	0.001%
79	9.792	2715	2722	2724	rBV2	443	474	0.03%	0.004%
80	9.834	2733	2735	2738	rVB3	519	246	0.02%	0.002%
81	9.882	2747	2750	2752	rBV	307	193	0.01%	0.002%
82	10.075	2808	2810	2813	rBV2	292	174	0.01%	0.001%
83	10.130	2819	2827	2834	rBV4	3210	4562	0.29%	0.036%
84	10.217	2842	2854	2877	rBV	494129	788709	49.68%	6.309%
85	10.352	2893	2896	2902	rVB6	787	639	0.04%	0.005%
86	10.506	2942	2944	2945	rBV	450	147	0.01%	0.001%
87	10.545	2952	2956	2960	rBV3	649	729	0.05%	0.006%
88	10.664	2989	2993	2998	rBV3	440	425	0.03%	0.003%
89	10.693	3000	3002	3005	rBV2	319	180	0.01%	0.001%
90	10.738	3013	3016	3017	rBV	396	218	0.01%	0.002%
91	10.779	3026	3029	3035	rBV2	440	440	0.03%	0.004%
92	10.921	3065	3073	3082	rVB5	3813	5706	0.36%	0.046%
93	10.982	3090	3092	3095	rVB	277	132	0.01%	0.001%
94	11.037	3102	3109	3116	rBV5	1212	1647	0.10%	0.013%
95	11.152	3136	3145	3154	rVB6	2331	3932	0.25%	0.031%
96	11.201	3154	3160	3163	rBV3	458	492	0.03%	0.004%
97	11.249	3163	3175	3196	rBV	750783	1189806	74.95%	9.518%
98	11.625	3280	3292	3311	rBV	740014	1179600	74.31%	9.436%
99	11.834	3355	3357	3360	rBV4	622	433	0.03%	0.003%
100	12.696	3623	3625	3629	rBV	389	186	0.01%	0.001%




Sum of corrected areas: 12500446

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021658.D
Acq On : 14 Jul 2021 17:12
Operator : SY/MD
Sample : M3033-09 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

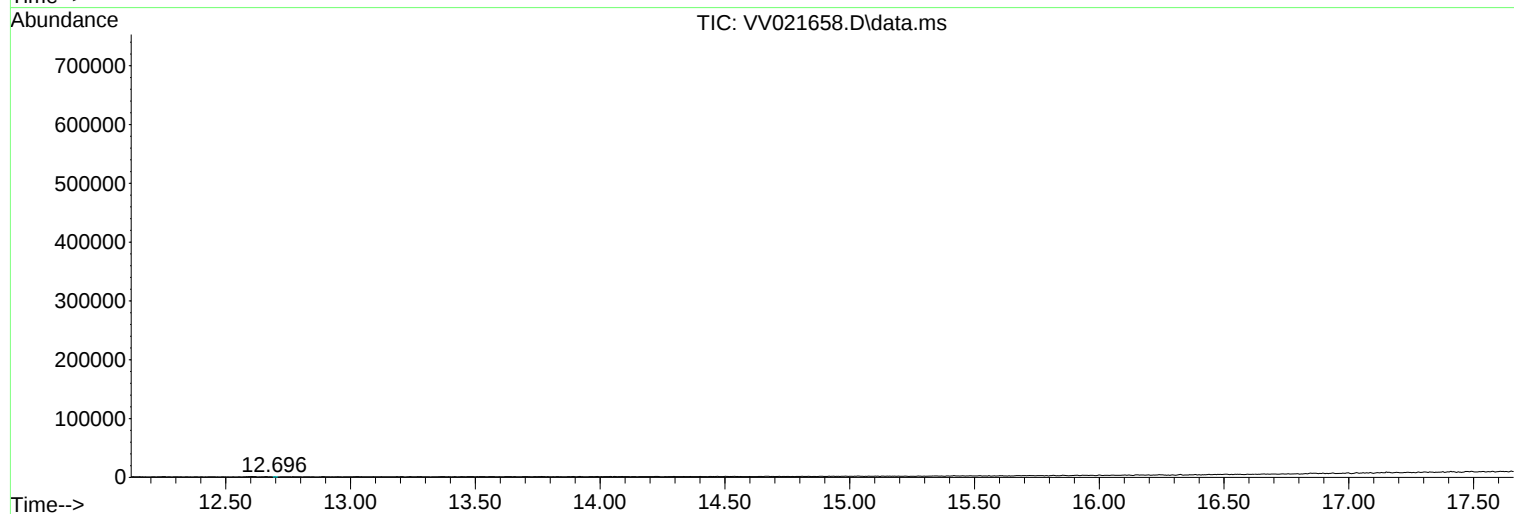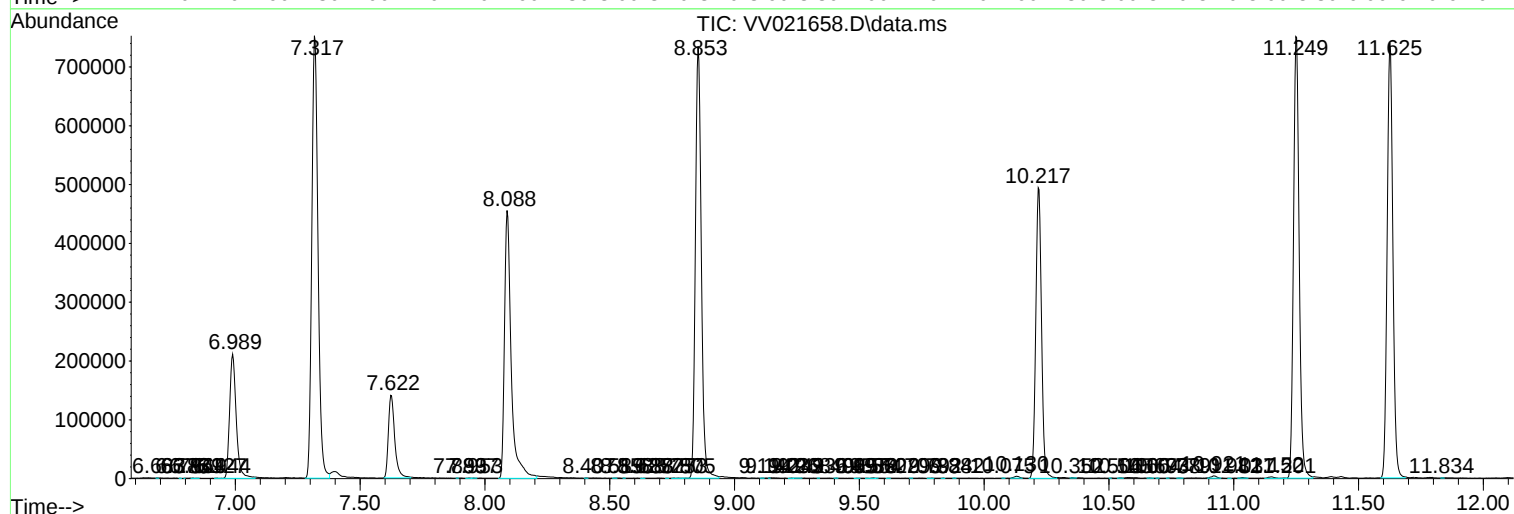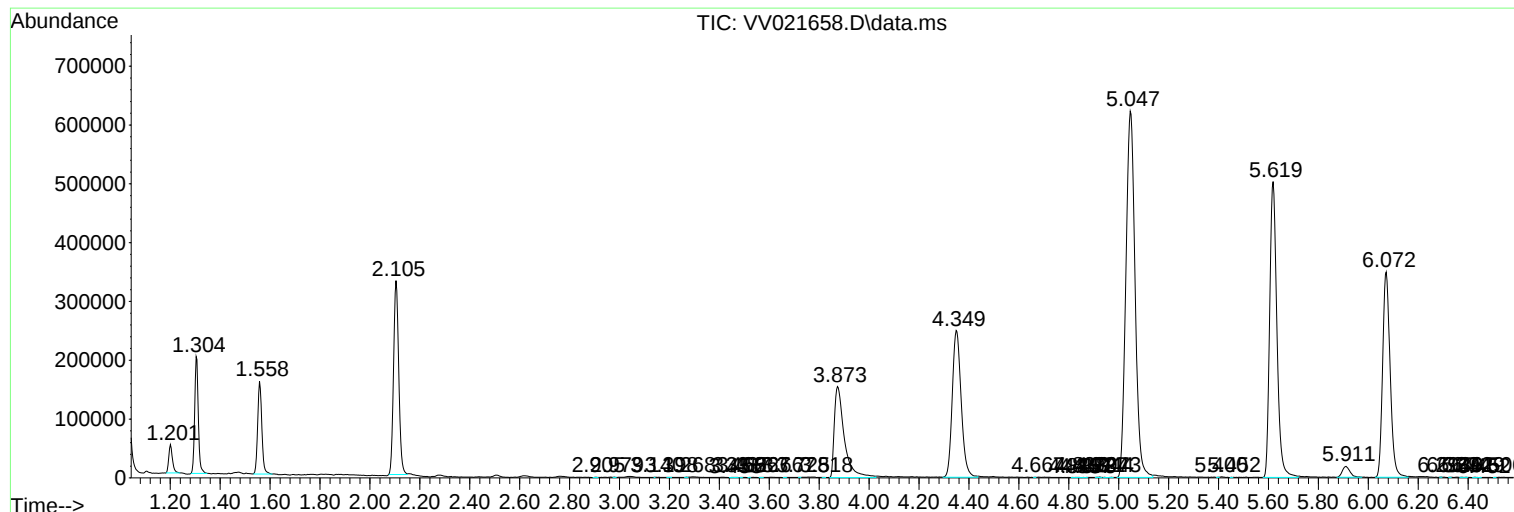

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021658.D
Acq On : 14 Jul 2021 17:12
Operator : SY/MD
Sample : M3033-09 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021658.D
Acq On : 14 Jul 2021 17:12
Operator : SY/MD
Sample : M3033-09 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
