
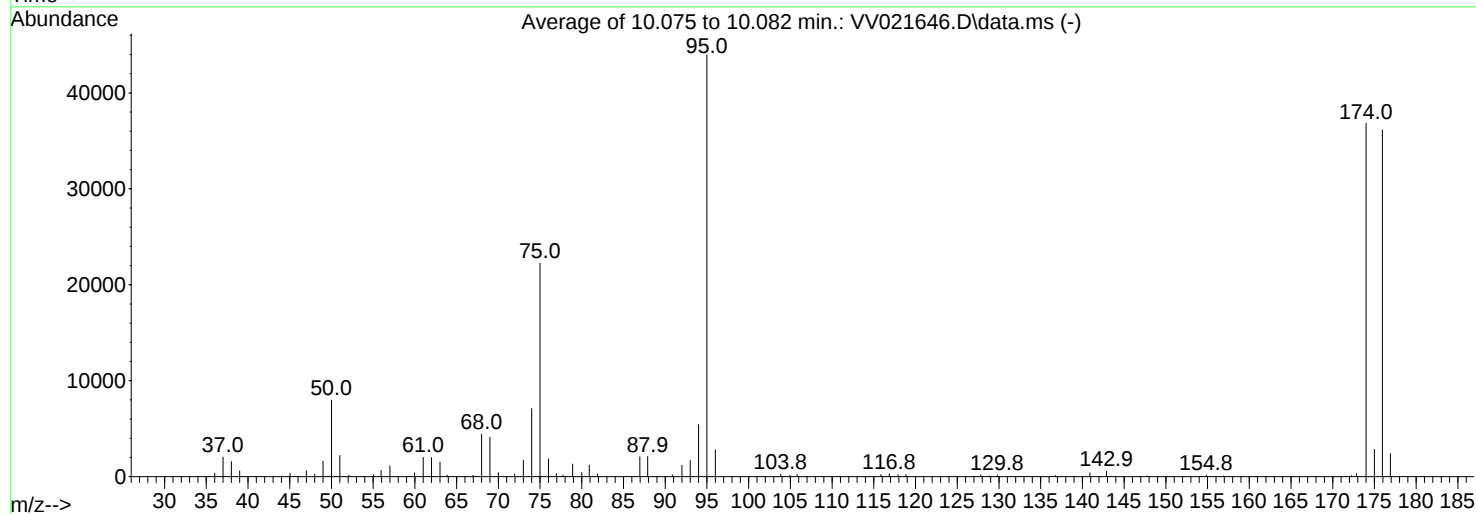


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071421\
Data File : VV021646.D
Acq On : 14 Jul 2021 09:33
Operator : SY/MD
Sample : BFB205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Title : VOC Analysis
Last Update : Fri Jul 16 01:06:31 2021

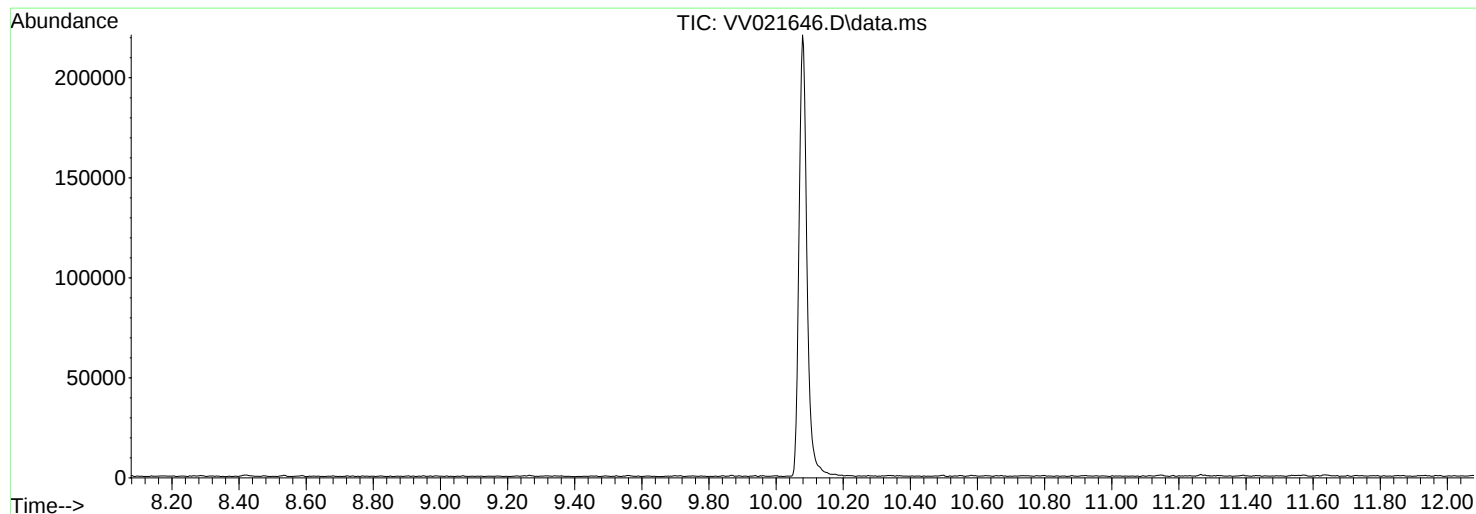

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	7979	PASS
75	95	30	80	50.6	22240	PASS
95	95	100	100	100.0	43965	PASS
96	95	5	9	6.4	2811	PASS
173	174	0.00	2	0.9	340	PASS
174	95	50	120	83.7	36816	PASS
175	174	5	9	7.7	2838	PASS
176	174	95	105	98.2	36141	PASS
177	176	5	10	6.6	2379	PASS

m/z	Abundance
36.00	345.0
37.00	1956.0
38.00	1445.0
39.00	629.0
39.90	190.0
40.90	109.0
44.00	755.0
45.00	303.0
47.00	619.0
48.00	243.0
49.00	1503.0
50.00	7735.0
51.00	2222.0
52.10	145.0
55.00	199.0
55.90	730.0
57.00	1086.0
59.90	397.0
61.00	1916.0
62.00	1932.0
63.00	1472.0
63.90	131.0
67.00	114.0
68.00	4310.0
69.00	4314.0
70.00	365.0
72.00	248.0
73.00	1596.0
74.00	7073.0
75.00	21272.0
76.00	1771.0
77.00	298.0
77.80	187.0
78.90	1344.0
80.00	439.0
80.90	1196.0
81.90	272.0
86.90	2037.0
87.90	2012.0
90.80	177.0
92.00	1095.0
93.00	1588.0
94.00	5242.0
95.00	42248.0
96.00	2760.0
103.80	229.0
104.90	123.0
105.80	215.0
115.80	186.0
116.90	242.0
117.90	196.0
118.90	187.0
127.80	154.0
128.90	107.0
129.80	156.0
136.80	113.0
140.90	412.0
142.90	542.0
147.80	102.0
154.80	184.0
160.80	106.0
172.80	282.0
174.00	34832.0
175.00	2603.0
175.90	34040.0
176.90	2251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Scan 2800 (10.043 min): VV021646.D\data.ms
BFB205

m/z	Abundance
39.90	193.0
44.00	657.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	377.0
37.00	2047.0
38.00	1682.0
39.00	560.0
39.90	234.0
44.00	710.0
45.00	343.0
47.00	593.0
48.00	276.0
49.00	1651.0
50.00	7858.0
51.00	2155.0
52.10	128.0
55.10	193.0
56.00	572.0
57.00	1158.0
60.00	420.0
61.00	2013.0
62.00	1977.0
63.00	1516.0
63.80	184.0
66.90	141.0
68.00	4435.0
69.00	3838.0
70.00	456.0
71.90	237.0
73.00	1804.0
74.00	6818.0
75.00	22312.0
76.00	1873.0
76.90	350.0
77.80	147.0
78.90	1257.0
80.00	402.0
80.90	1118.0
81.90	292.0
85.90	107.0
87.00	2015.0
87.90	2089.0
90.90	208.0
92.00	1251.0
93.00	1721.0
94.00	5360.0
95.00	44336.0
96.00	2780.0
103.90	225.0
105.00	110.0
105.80	211.0
115.90	248.0
116.80	359.0
117.90	209.0
118.80	202.0
127.80	173.0
129.80	192.0
136.80	105.0
140.90	374.0
142.90	581.0
154.90	118.0
156.90	123.0
172.20	202.0
172.90	379.0
174.00	37568.0
175.00	2984.0
176.00	37112.0
176.90	2422.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	373.0
37.00	2113.0
38.00	1589.0
39.00	593.0
39.90	226.0
44.00	748.0
45.10	349.0
47.00	618.0
48.00	268.0
49.00	1689.0
50.00	8344.0
51.00	2237.0
52.10	151.0
55.10	210.0
56.00	640.0
57.00	1135.0
60.00	408.0
61.00	2090.0
62.00	2045.0
63.00	1590.0
63.80	164.0
67.00	126.0
68.00	4580.0
69.00	4164.0
70.00	433.0
72.00	262.0
73.00	1723.0
74.00	7389.0
75.00	23136.0
76.00	1895.0
76.90	326.0
77.70	176.0
78.90	1363.0
80.00	448.0
80.90	1269.0
81.90	288.0
86.90	2164.0
87.90	2194.0
90.80	183.0
92.00	1214.0
93.00	1741.0
94.00	5673.0
95.00	45312.0
96.00	2893.0
103.80	249.0
105.00	124.0
105.80	223.0
115.80	224.0
116.80	297.0
117.90	231.0
118.80	193.0
127.80	173.0
128.90	119.0
129.80	184.0
136.70	115.0
140.90	410.0
142.90	591.0
147.70	111.0
154.80	160.0
156.90	115.0
160.80	110.0
172.30	147.0
172.90	360.0
174.00	38048.0
175.00	2927.0
176.00	37272.0
176.90	2464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205