




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026779.D
 Acq On : 14 Jul 2022 15:56
 Operator : SY/MD
 Sample : N3709-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:44:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 15 06:40:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

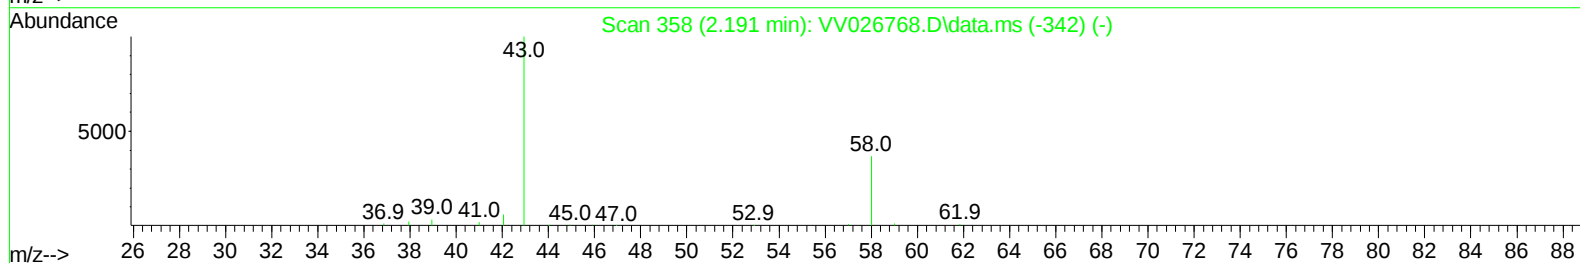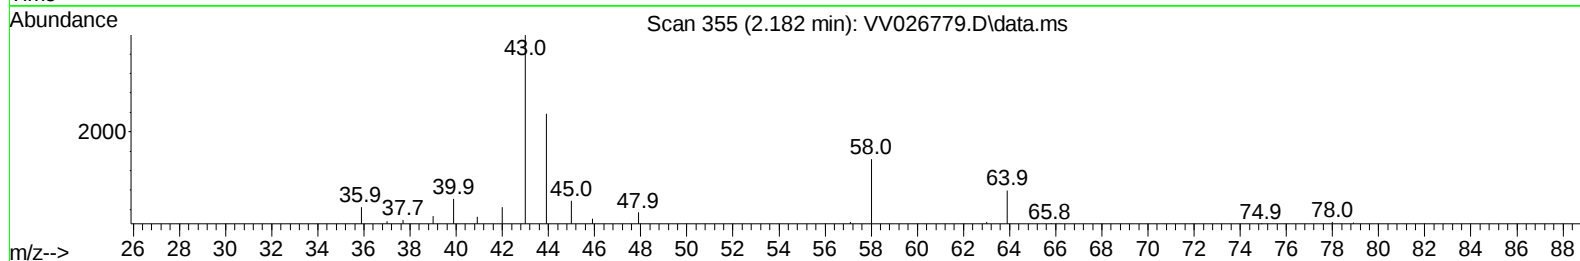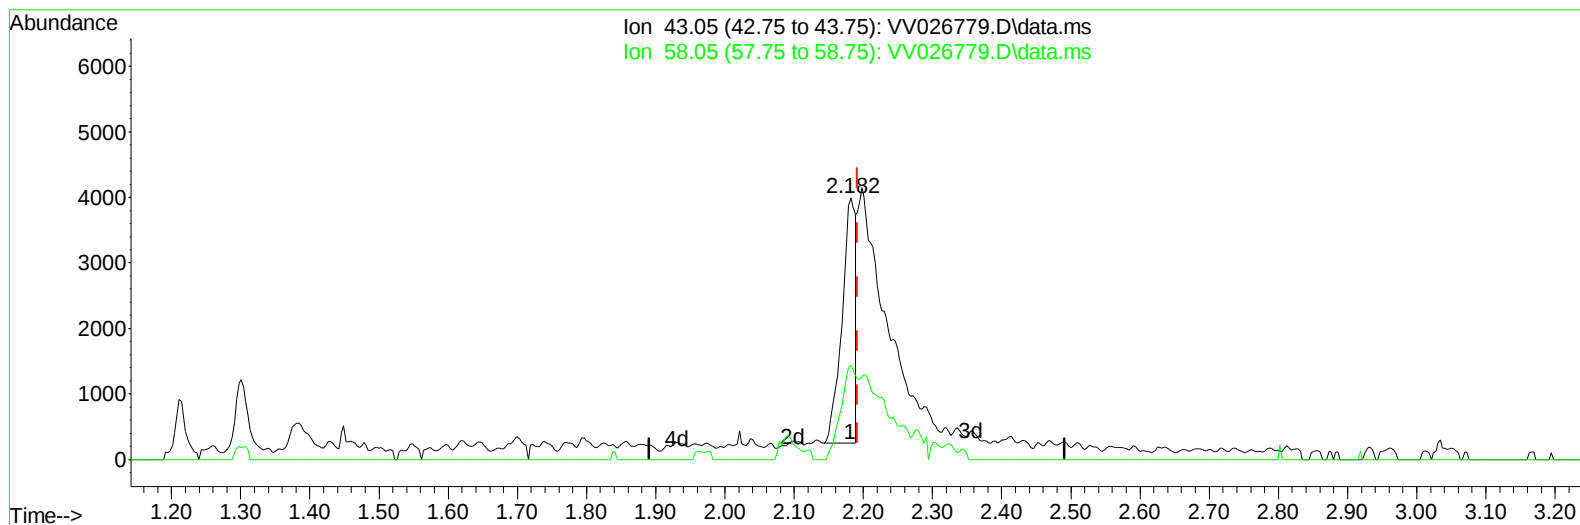

TIC: VV026779.D\data.ms

(13) Acetone (T)

2.182min (-0.010) 1.90 ug/L

response 5033

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	10.30	50.71#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026779.D
 Acq On : 14 Jul 2022 15:56
 Operator : SY/MD
 Sample : N3709-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:44:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 15 06:40:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

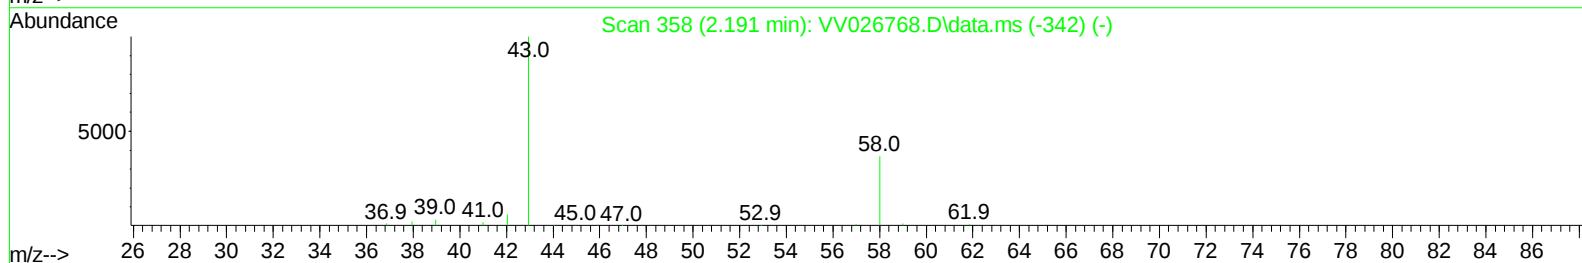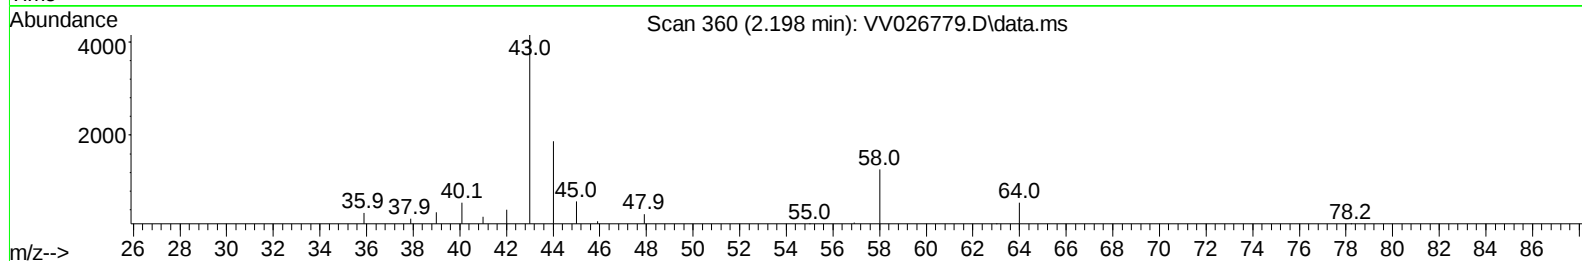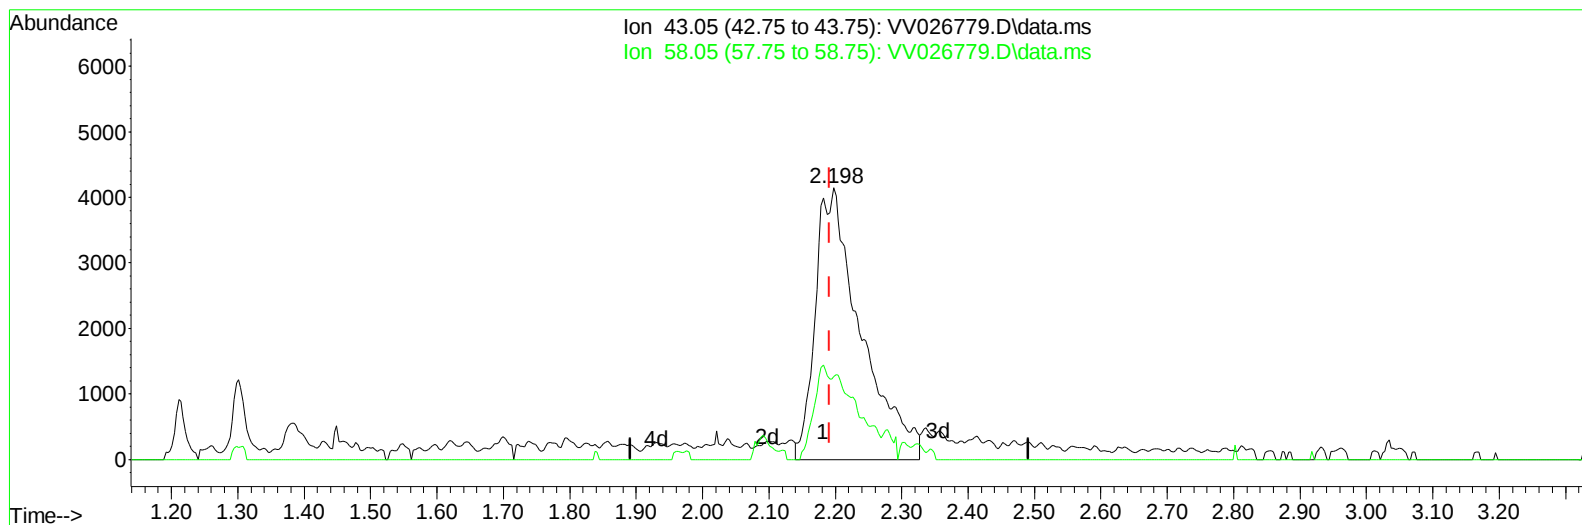

TIC: VV026779.D\data.ms

(13) Acetone (T)

2.198min (+ 0.006) 7.39 ug/L m

response 19607

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	10.30	13.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026779.D
 Acq On : 14 Jul 2022 15:56
 Operator : SY/MD
 Sample : N3709-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:44:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 15 06:40:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		221409	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		225861	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		89647	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		66153	3.275	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.600%	
7) Chloroethane-d5	1.561	69		67745	3.882	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.600%	
11) 1,1-Dichloroethene-d2	2.101	63		96044	2.477	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.600%#	
20) 2-Butanone-d5	3.899	46		166852	52.927	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.860%	
24) Chloroform-d	4.346	84		153143	4.336	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.031	65		69472	4.502	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%	
32) Benzene-d6	5.047	84		255328	3.720	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.400%	
36) 1,2-Dichloropropane-d6	6.066	67		90448	4.395	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.000%	
41) Toluene-d8	7.313	98		180892	2.969	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	59.400%#	
43) trans-1,3-Dichloroprop...	7.625	79		23021	3.419	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.400%	
46) 2-Hexanone-d5	8.088	63		127553	43.759	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		71518	4.461	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		70277	4.499	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.000%	
Target Compounds							
13) Acetone	2.198	43		19607m	7.392	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
Data File : VV026779.D
Acq On : 14 Jul 2022 15:56
Operator : SY/MD
Sample : N3709-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
H0B52

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:44:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 15 06:40:32 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

