

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026769.D
 Acq On : 14 Jul 2022 11:35
 Operator : SY/MD
 Sample : VV0714WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK394

Quant Time: Jul 15 06:41:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 15 06:40:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	219738	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	224196	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	88948	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	119407	5.957	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	119.200%	
7) Chloroethane-d5	1.561	69	100694	5.813	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	116.200%	
11) 1,1-Dichloroethene-d2	2.098	63	169874	4.414	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	88.200%	
20) 2-Butanone-d5	3.908	46	137168	43.842	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.680%	
24) Chloroform-d	4.342	84	198795	5.671	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	113.400%	
26) 1,2-Dichloroethane-d4	5.031	65	90447	5.906	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	118.200%	
32) Benzene-d6	5.043	84	375254	5.508	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.200%	
36) 1,2-Dichloropropane-d6	6.066	67	118037	5.779	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	115.600%	
41) Toluene-d8	7.313	98	286237	4.733	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.600%	
43) trans-1,3-Dichloroprop...	7.622	79	31774	4.755	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.000%	
46) 2-Hexanone-d5	8.088	63	138716	47.943	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.880%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	82293	5.172	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	90436	5.835	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	116.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	17816	0.776	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
Data File : VV026769.D
Acq On : 14 Jul 2022 11:35
Operator : SY/MD
Sample : VV0714WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK394


Quant Time: Jul 15 06:41:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 15 06:40:32 2022
Response via : Initial Calibration

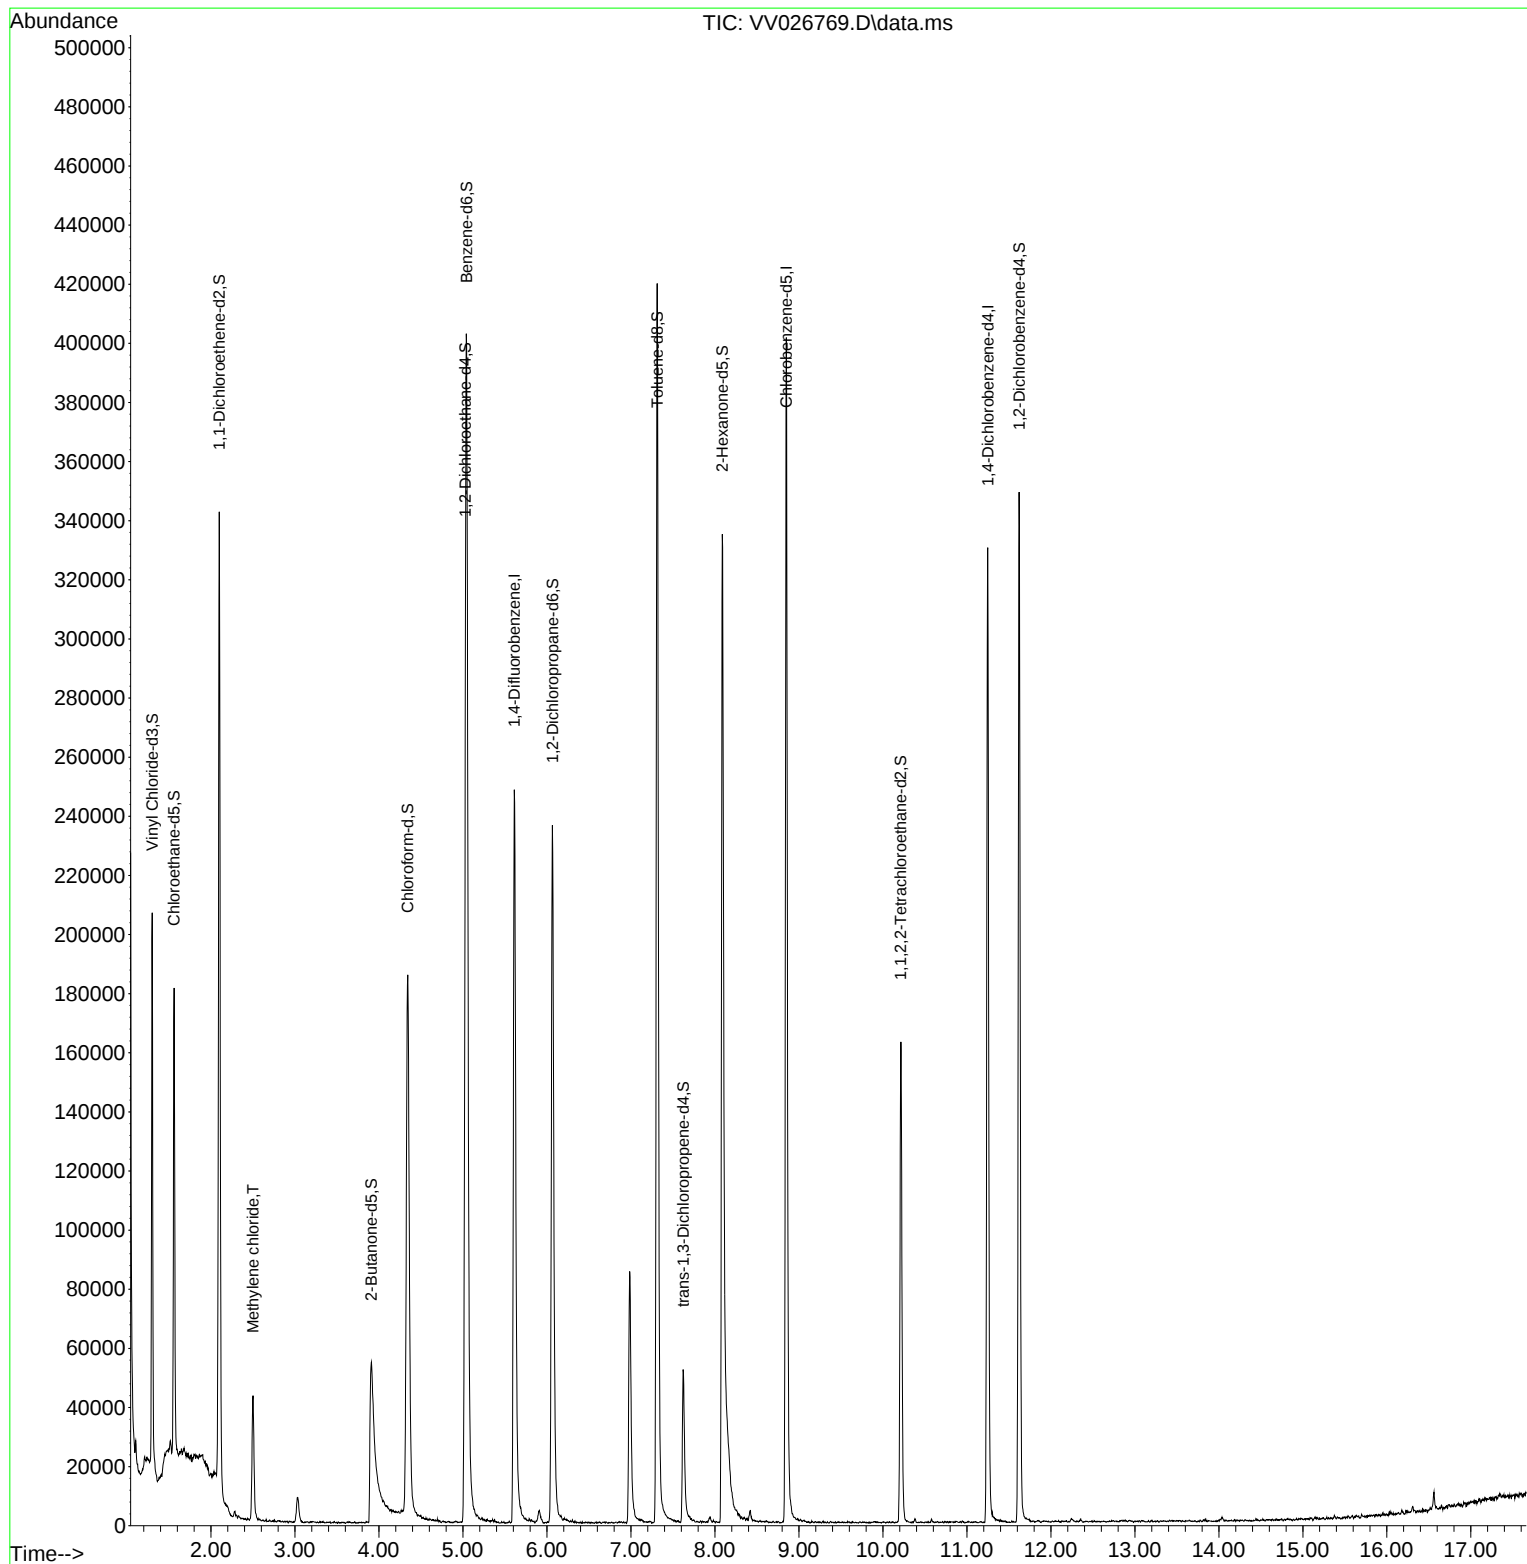

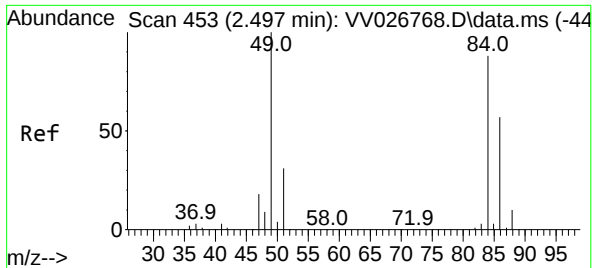

#16
Methylene chloride
Concen: 0.776 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026769.D
Acq: 14 Jul 2022 11:35

Instrument :
MSVOA_V
ClientSampleId :
VBLK394

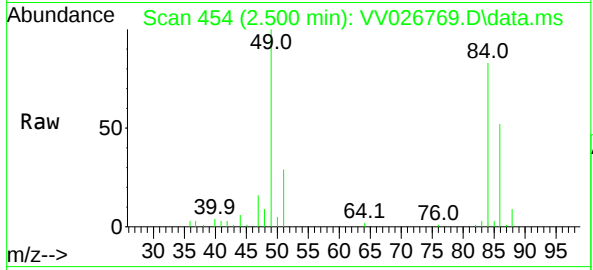

Tgt Ion:	84	Resp:	17816
Ion	Ratio	Lower	Upper
84	100		
86	63.1	44.8	83.2
49	120.5	78.7	146.1

