

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026775.D
 Acq On : 14 Jul 2022 14:07
 Operator : SY/MD
 Sample : N3658-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Quant Time: Jul 15 06:43:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 15 06:40:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	208499	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	217320	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	85103	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	115170	6.055	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	121.000%	
7) Chloroethane-d5	1.561	69	97701	5.945	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	118.800%	
11) 1,1-Dichloroethene-d2	2.098	63	162450	4.449	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	89.000%	
20) 2-Butanone-d5	3.908	46	158522	53.398	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.800%	
24) Chloroform-d	4.342	84	194098	5.836	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.800%	
26) 1,2-Dichloroethane-d4	5.031	65	86797	5.974	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	119.400%	
32) Benzene-d6	5.047	84	365982	5.542	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.800%	
36) 1,2-Dichloropropane-d6	6.066	67	115394	5.828	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	116.600%	
41) Toluene-d8	7.313	98	275722	4.704	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.000%	
43) trans-1,3-Dichloroprop...	7.625	79	30257	4.671	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.400%	
46) 2-Hexanone-d5	8.091	63	136516	48.675	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	79559	5.158	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	88297	5.955	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	119.000%	
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	7920	0.364	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
Data File : VV026775.D
Acq On : 14 Jul 2022 14:07
Operator : SY/MD
Sample : N3658-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002


Quant Time: Jul 15 06:43:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 15 06:40:32 2022
Response via : Initial Calibration

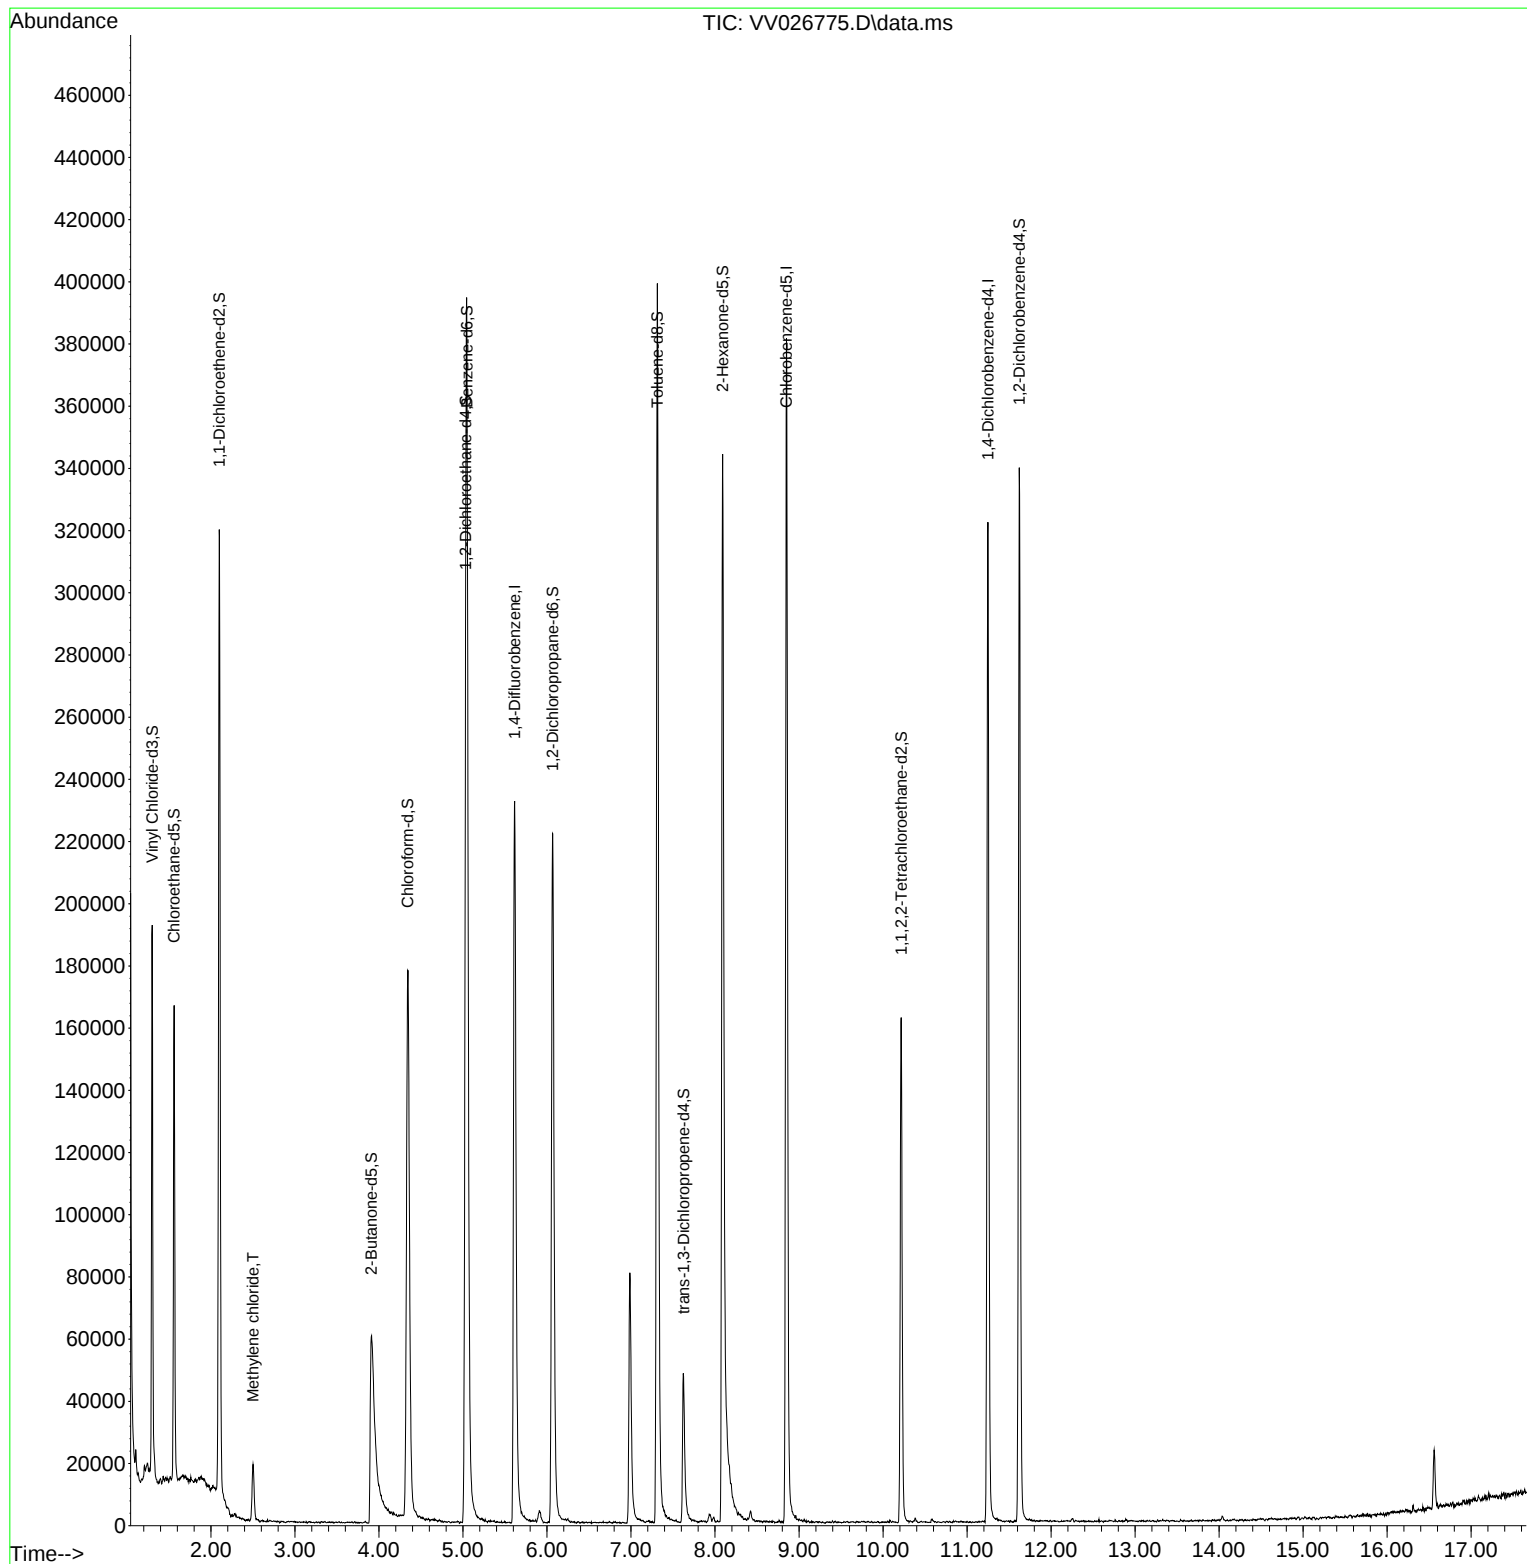

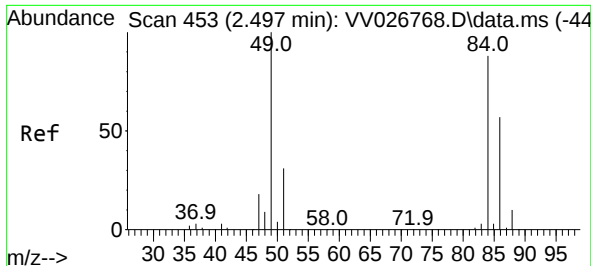

#16
Methylene chloride
Concen: 0.364 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV026775.D
Acq: 14 Jul 2022 14:07

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

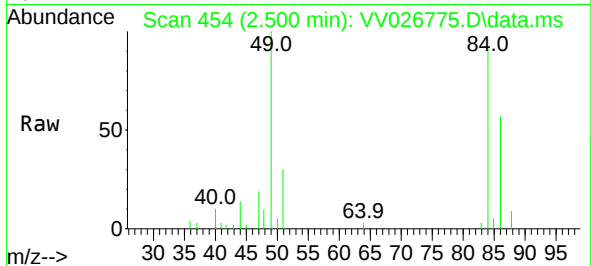

Tgt Ion: 84 Resp: 7920

Ion	Ratio	Lower	Upper
84	100		
86	62.6	44.8	83.2
49	110.4	78.7	146.1

