

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026779.D
 Acq On : 14 Jul 2022 15:56
 Operator : SY/MD
 Sample : N3709-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B52

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Quant Time: Jul 15 06:44:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jul 15 06:40:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	221409	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	225861	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	89647	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	66153	3.275	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	65.600%	
7) Chloroethane-d5	1.561	69	67745	3.882	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	77.600%	
11) 1,1-Dichloroethene-d2	2.101	63	96044	2.477	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	49.600%#	
20) 2-Butanone-d5	3.899	46	166852	52.927	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.860%	
24) Chloroform-d	4.346	84	153143	4.336	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.031	65	69472	4.502	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.000%	
32) Benzene-d6	5.047	84	255328	3.720	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	74.400%	
36) 1,2-Dichloropropane-d6	6.066	67	90448	4.395	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.000%	
41) Toluene-d8	7.313	98	180892	2.969	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	59.400%#	
43) trans-1,3-Dichloroprop...	7.625	79	23021	3.419	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	68.400%	
46) 2-Hexanone-d5	8.088	63	127553	43.759	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	71518	4.461	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	89.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	70277	4.499	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	90.000%	
Target Compounds					Qvalue	
13) Acetone	2.198	43	19607m	7.392	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
Data File : VV026779.D
Acq On : 14 Jul 2022 15:56
Operator : SY/MD
Sample : N3709-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
H0B52

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022


Quant Time: Jul 15 06:44:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jul 15 06:40:32 2022
Response via : Initial Calibration

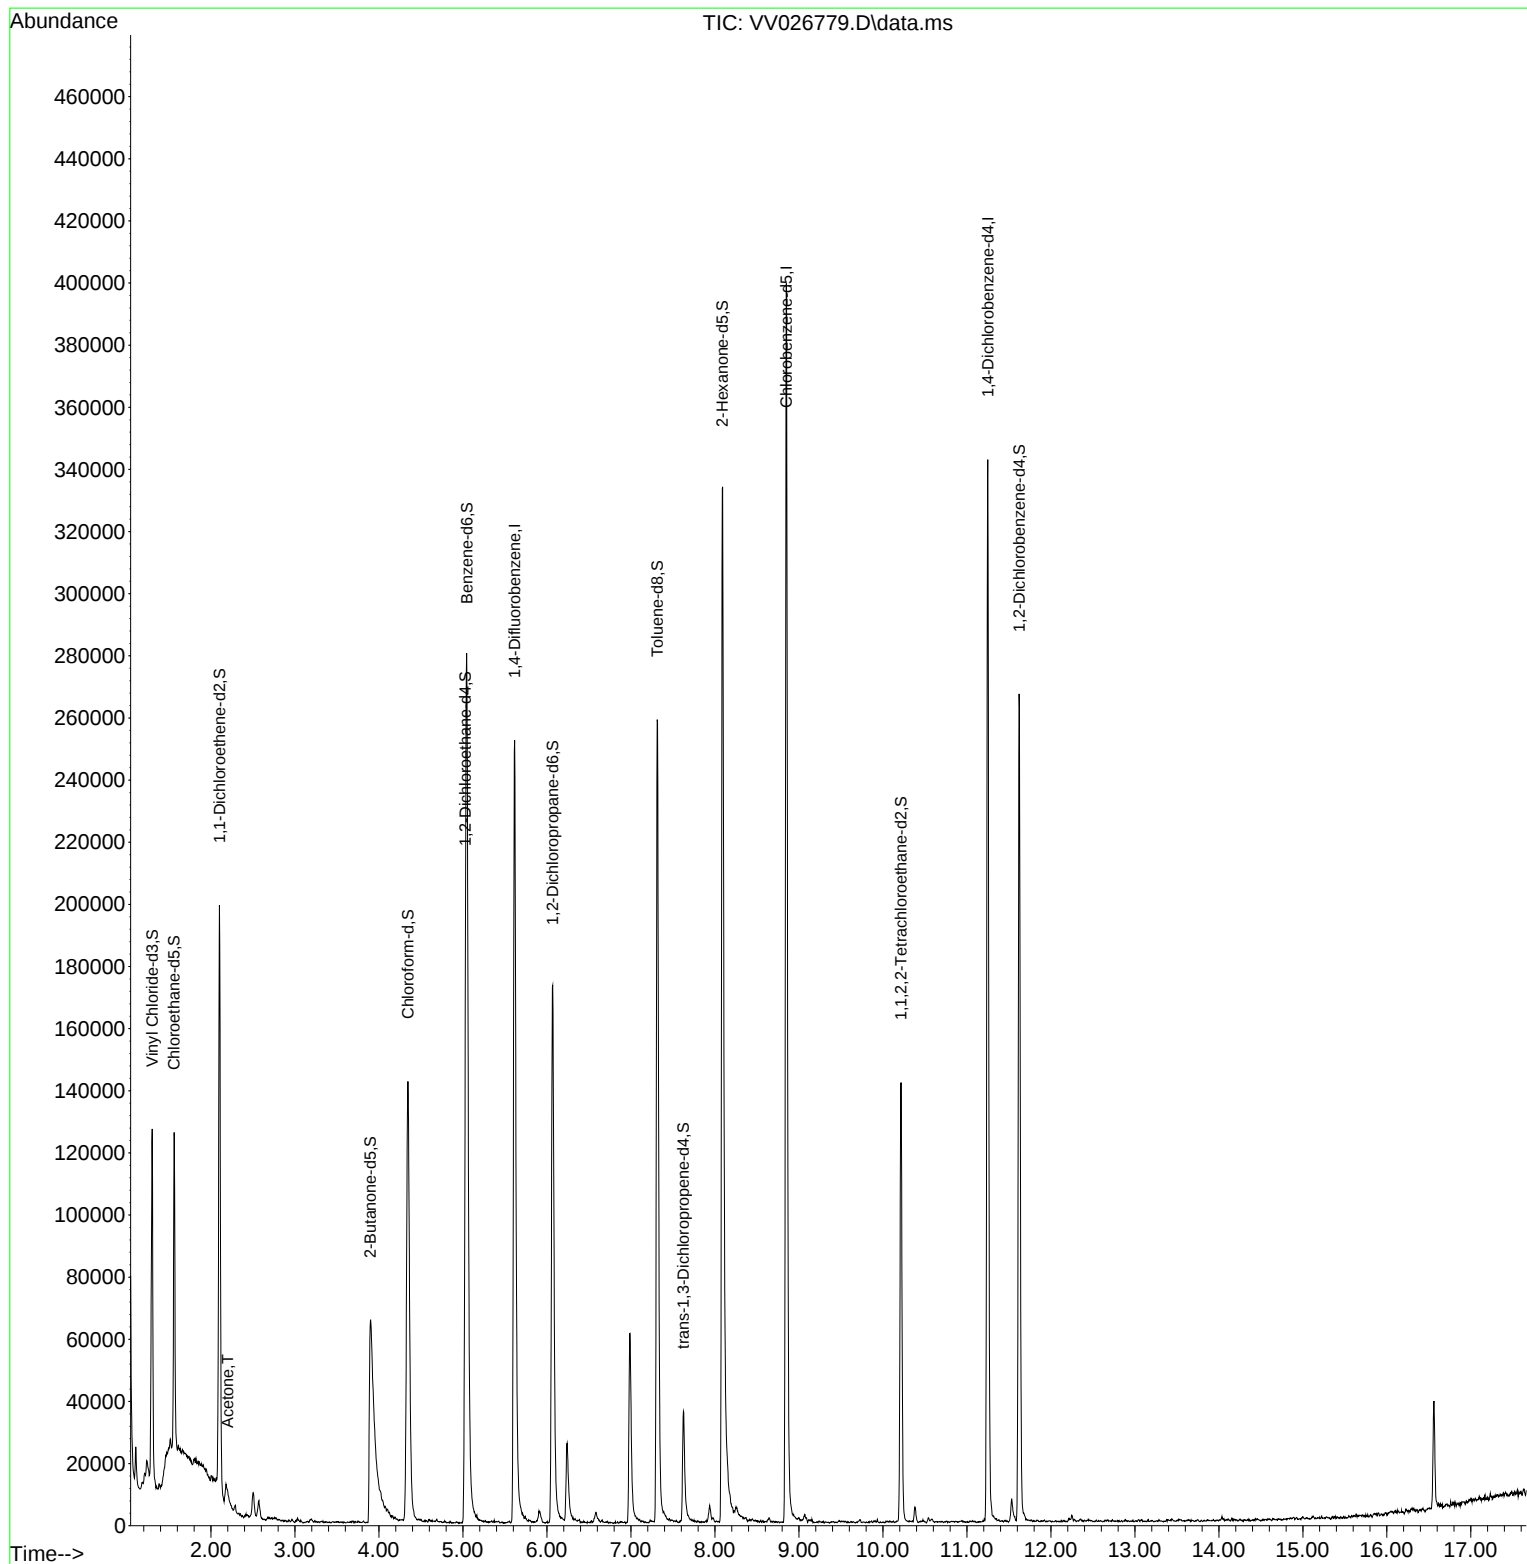

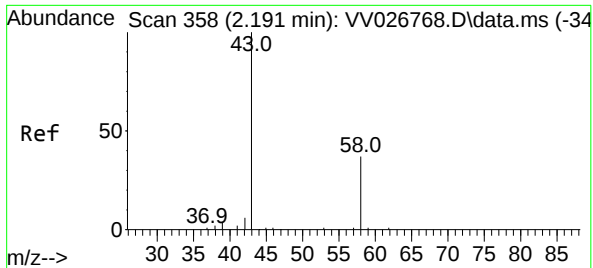

#13
 Acetone
 Concen: 7.392 ug/L m
 RT: 2.198 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VV026779.D
 Acq: 14 Jul 2022 15:56

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B52

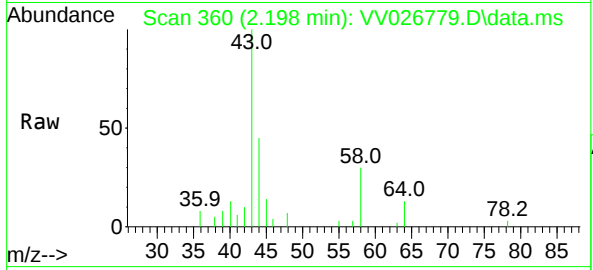

Tgt Ion: 43 Resp: 1960

Ion	Ratio	Lower	Upper
43	100		
58	13.0	0.0	20.6

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

