
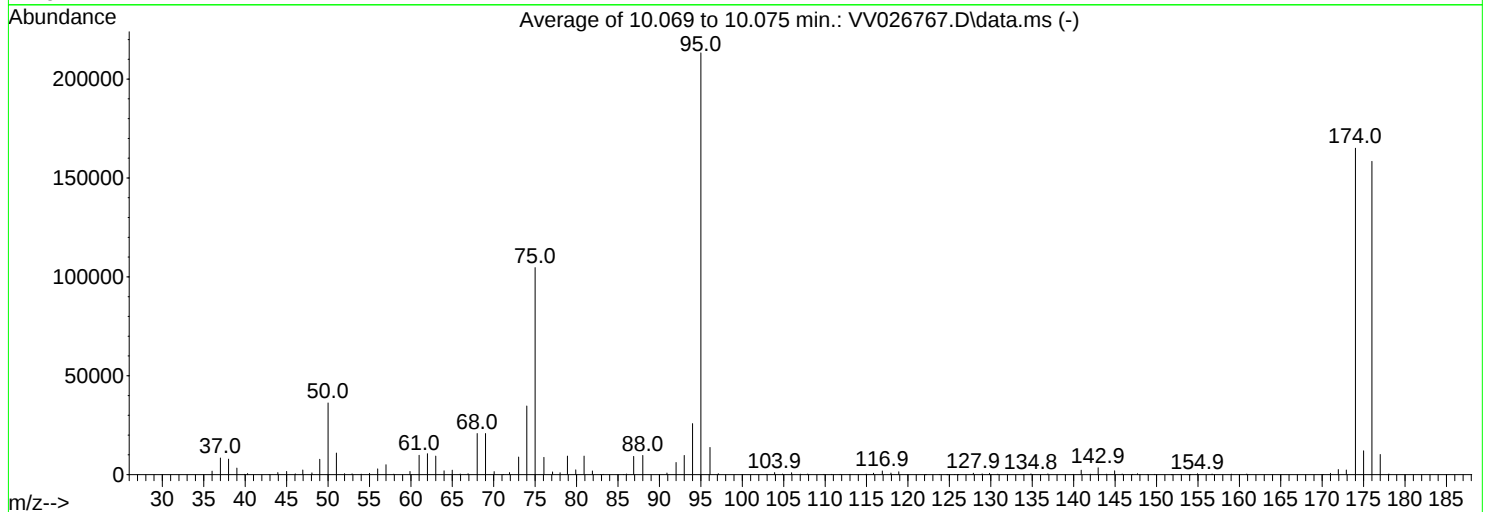


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071422\
 Data File : VV026767.D
 Acq On : 14 Jul 2022 08:45
 Operator : SY/MD
 Sample : BFB345
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB345

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jul 15 06:40:32 2022

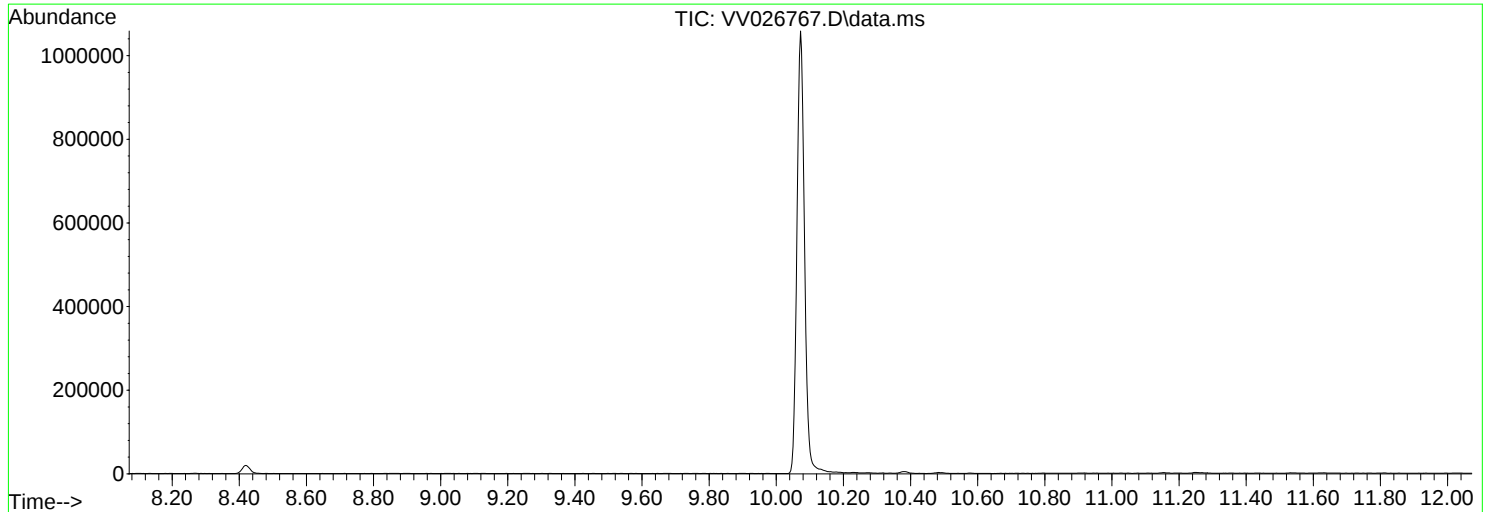

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	36245	PASS
75	95	30	80	49.1	104709	PASS
95	95	100	100	100.0	213269	PASS
96	95	5	9	6.5	13775	PASS
173	174	0.00	2	1.4	2368	PASS
174	95	50	120	77.4	165035	PASS
175	174	5	9	7.3	12033	PASS
176	174	95	105	96.0	158379	PASS
177	176	5	10	6.4	10206	PASS

m/z	Abundance
39.90	367.0
44.00	499.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345

m/z	Abundance
36.00	1755.0
37.00	8571.0
38.00	7640.0
39.00	3257.0
39.90	565.0
40.30	672.0
43.90	1462.0
45.00	1645.0
46.10	447.0
46.90	2196.0
48.00	923.0
49.00	7566.0
50.00	35824.0
51.00	10619.0
52.00	475.0
52.90	274.0
54.00	229.0
55.00	715.0
56.00	2929.0
57.00	5069.0
58.00	232.0
59.90	1656.0
61.00	9798.0
62.00	10187.0
63.00	9524.0
64.00	2140.0
65.00	2295.0
65.90	316.0
66.80	458.0
68.00	20424.0
69.00	20376.0
70.00	1567.0
71.10	140.0
71.90	1057.0
73.00	8678.0
74.00	34920.0
75.00	102888.0
76.00	8745.0
77.10	1520.0
78.00	960.0
78.90	9388.0
79.90	2420.0
80.90	9376.0
81.90	1765.0
83.20	267.0
85.70	309.0
86.00	290.0
86.90	9218.0
88.00	9474.0
90.90	752.0
92.00	5993.0
93.00	9448.0
94.00	24720.0
95.00	208704.0
96.10	13401.0
97.10	511.0
102.90	129.0
103.90	1054.0
104.90	386.0
106.00	965.0
107.00	244.0
107.90	355.0
109.90	157.0
110.80	225.0
111.80	174.0
113.00	177.0
114.90	200.0
115.90	708.0
116.90	1887.0
118.00	756.0
118.90	1426.0
122.10	110.0
125.80	104.0
127.90	715.0
129.00	387.0
129.90	662.0
130.80	253.0
134.80	382.0
136.90	461.0
140.00	174.0
140.90	1965.0
142.00	219.0
143.00	3338.0
144.00	239.0
144.90	1986.0
145.90	367.0
147.10	126.0
147.70	397.0
148.00	367.0
148.90	115.0
149.80	167.0
151.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345

152.90	170.0
153.80	114.0
154.90	524.0
156.70	340.0
159.10	237.0
160.90	423.0
171.00	641.0
172.00	2505.0
172.90	2097.0
174.00	157568.0
175.00	11650.0
176.00	150912.0
177.00	9901.0
178.10	288.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345

m/z	Abundance
36.00	1853.0
37.00	8674.0
38.00	8145.0
39.00	3483.0
39.90	499.0
40.30	632.0
42.90	115.0
44.00	1564.0
45.00	1668.0
46.00	385.0
47.00	2430.0
48.10	899.0
49.00	8012.0
50.00	37544.0
51.00	11221.0
52.00	492.0
52.90	359.0
54.00	240.0
55.00	628.0
56.00	3049.0
57.00	5251.0
57.90	232.0
59.90	1702.0
61.00	10109.0
62.00	11035.0
63.00	9769.0
64.00	1959.0
65.00	2461.0
65.90	304.0
66.90	486.0
68.00	21528.0
69.00	21584.0
70.00	1537.0
71.20	130.0
71.90	1102.0
73.00	9206.0
74.00	35728.0
75.00	108472.0
76.00	9115.0
77.10	1446.0
78.00	1046.0
78.90	9689.0
79.90	2472.0
80.90	9772.0
81.90	1966.0
83.20	300.0
86.10	323.0
86.90	9450.0
88.00	10169.0
90.90	828.0
92.00	6280.0
93.00	10038.0
94.00	26744.0
95.00	221184.0
96.10	14246.0
97.10	528.0
102.90	136.0
103.90	1084.0
104.80	390.0
106.00	1011.0
107.10	256.0
107.90	345.0
109.80	142.0
110.80	211.0
111.80	156.0
113.00	191.0
115.00	203.0
115.80	763.0
116.90	1926.0
117.90	857.0
118.90	1462.0
123.80	144.0
124.70	104.0
125.60	106.0
126.00	102.0
127.90	757.0
129.00	437.0
129.80	697.0
130.90	285.0
134.90	379.0
136.90	443.0
139.00	109.0
139.90	196.0
140.90	2359.0
142.00	246.0
142.90	3608.0
144.00	251.0
145.00	2069.0
145.90	327.0
147.10	155.0
147.70	513.0
148.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345

149.80	209.0
152.90	170.0
153.80	135.0
154.90	511.0
156.70	385.0
159.10	218.0
160.90	381.0
170.10	124.0
171.00	700.0
172.00	2723.0
172.90	2498.0
174.00	170880.0
175.00	12509.0
176.00	163904.0
177.00	10495.0
178.10	325.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345

m/z	Abundance
36.00	1640.0
37.00	8000.0
38.00	7717.0
39.00	3332.0
39.90	464.0
40.30	504.0
42.90	122.0
44.00	1607.0
45.00	1466.0
46.00	304.0
47.00	2461.0
48.00	831.0
49.00	7775.0
50.00	35368.0
51.00	10840.0
52.00	481.0
52.90	473.0
54.00	255.0
55.00	521.0
56.00	2882.0
57.00	4744.0
57.90	271.0
59.90	1625.0
61.00	9482.0
62.00	10709.0
63.00	8816.0
64.00	1751.0
65.00	2162.0
66.00	278.0
67.00	431.0
68.00	20560.0
69.00	20536.0
70.10	1494.0
71.90	1111.0
73.00	8796.0
74.00	33376.0
75.00	102768.0
76.10	8487.0
77.10	1163.0
78.00	980.0
78.90	9063.0
79.90	2353.0
80.90	9026.0
81.90	1943.0
82.90	308.0
86.10	314.0
86.90	9088.0
88.00	9488.0
90.90	843.0
92.00	6084.0
93.00	9629.0
94.00	26064.0
95.00	209920.0
96.10	13679.0
97.10	492.0
102.90	149.0
103.90	1018.0
104.90	316.0
105.90	976.0
107.00	245.0
107.90	306.0
109.80	136.0
110.80	161.0
111.80	131.0
113.00	189.0
115.00	221.0
115.80	709.0
116.90	1827.0
117.90	890.0
118.90	1421.0
123.80	164.0
125.60	110.0
127.90	709.0
128.90	423.0
129.90	702.0
130.90	300.0
133.90	104.0
134.90	382.0
136.90	362.0
139.00	137.0
139.90	189.0
140.90	2449.0
142.00	261.0
142.90	3458.0
143.90	264.0
145.00	1852.0
145.80	290.0
147.10	159.0
147.70	533.0
148.90	111.0
149.80	236.0
153.00	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345

154.00	120.0
155.00	445.0
156.70	349.0
159.00	206.0
160.90	265.0
170.10	119.0
171.00	671.0
171.90	2662.0
172.90	2509.0
174.00	166656.0
175.00	11941.0
176.00	160320.0
177.00	10221.0
178.00	355.0

Instrument :
MSVOA_V
ClientSampleId :
BFB345