


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071423\
Data File : VV031701.D
Acq On : 14 Jul 2023 08:45
Operator : SY/MD
Sample : BFB282
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB282

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jul 15 05:25:11 2023

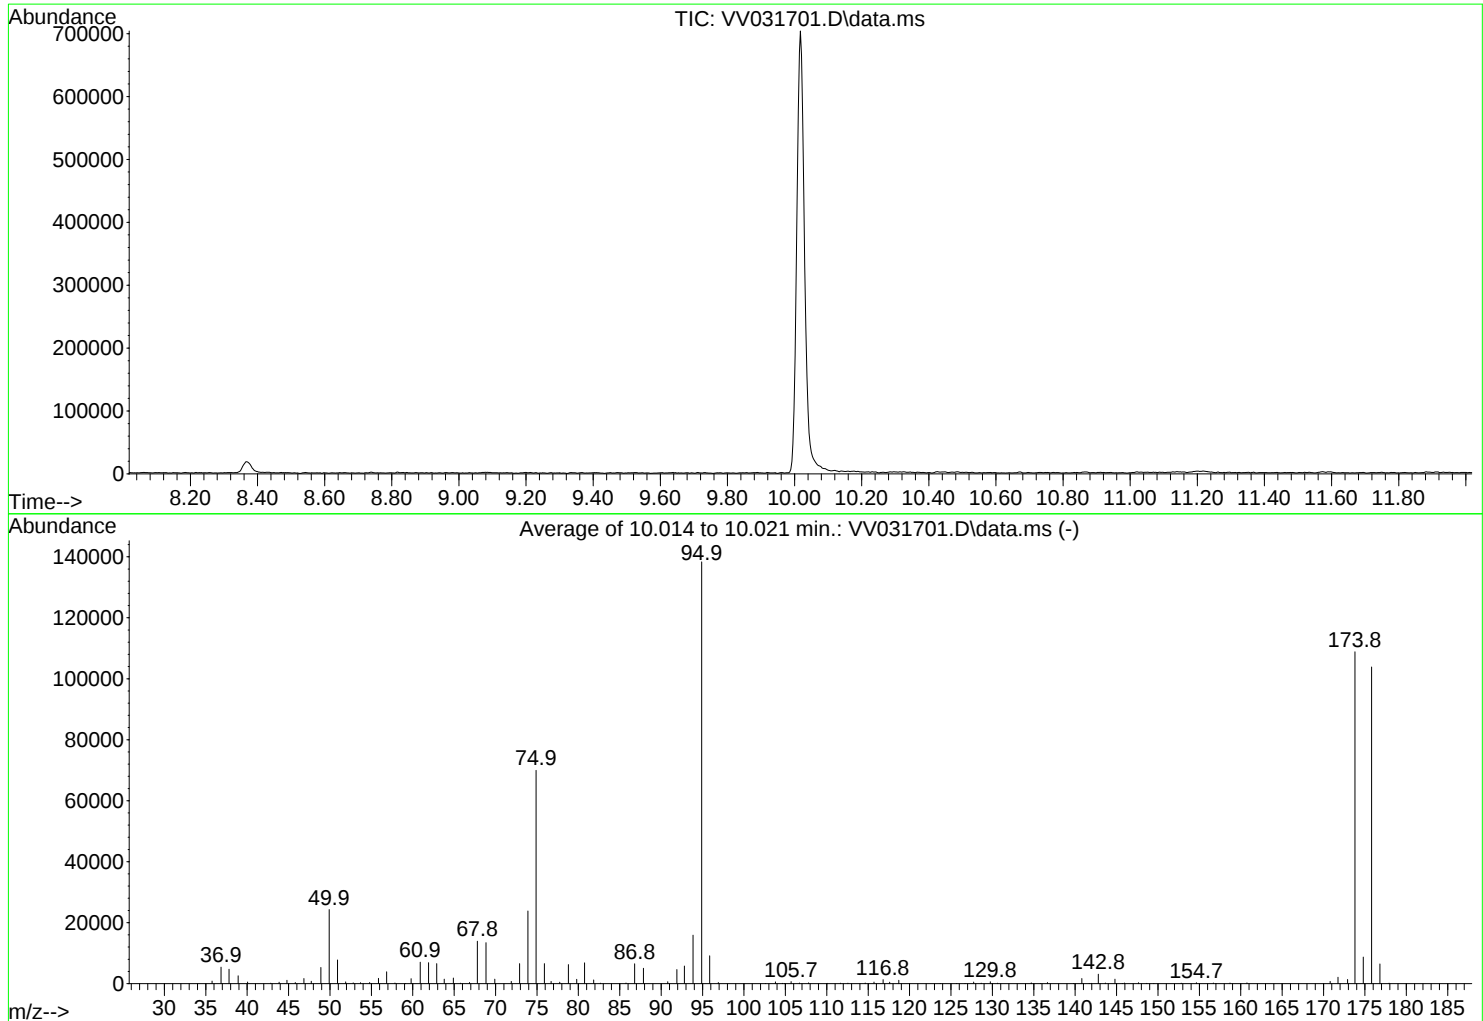

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	24291	PASS
75	95	30	80	50.6	69973	PASS
95	95	100	100	100.0	138347	PASS
96	95	5	9	6.6	9143	PASS
173	174	0.00	2	1.3	1362	PASS
174	95	50	120	78.7	108851	PASS
175	174	5	9	8.0	8719	PASS
176	174	95	105	95.4	103859	PASS
177	176	5	10	6.2	6458	PASS

m/z	Abundance
35.60	119.0
37.70	114.0
38.60	142.0
39.80	255.0
43.80	872.0
46.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.80	1111.0
36.90	5293.0
37.90	4834.0
38.90	2748.0
40.00	557.0
42.90	132.0
43.90	1217.0
44.80	1173.0
45.80	388.0
46.80	1830.0
47.70	834.0
48.90	5146.0
49.90	24984.0
50.90	8052.0
51.90	601.0
52.80	273.0
53.70	322.0
54.80	394.0
55.80	1714.0
56.90	3761.0
57.90	246.0
59.80	1583.0
60.90	6847.0
61.90	6826.0
62.90	6082.0
63.80	1317.0
64.90	1496.0
65.80	133.0
66.90	345.0
67.80	13791.0
68.90	13801.0
69.90	1603.0
71.90	786.0
72.90	6529.0
73.90	24104.0
74.90	69008.0
75.90	6504.0
76.70	713.0
77.80	446.0
78.80	6120.0
79.80	1357.0
80.70	6582.0
81.90	1118.0
82.70	180.0
85.70	201.0
86.80	6103.0
87.90	4906.0
90.80	655.0
91.90	4606.0
92.80	6021.0
93.80	16480.0
94.90	137088.0
95.80	9404.0
96.90	435.0
103.80	542.0
104.60	153.0
105.70	694.0
106.70	308.0
107.80	224.0
110.10	121.0
111.70	172.0
112.50	175.0
114.70	247.0
115.60	431.0
116.80	1255.0
117.60	458.0
118.70	1232.0
123.70	108.0
126.70	117.0
127.70	582.0
128.60	179.0
129.80	663.0
130.60	133.0
134.70	218.0
136.60	319.0
140.80	1850.0
142.00	205.0
142.80	3025.0
143.70	213.0
144.80	1545.0
145.70	233.0
147.60	261.0
148.60	150.0
152.80	144.0
154.70	225.0
156.70	265.0
158.70	210.0
160.70	208.0
170.80	743.0
171.70	1671.0
172.90	1996.0
173.80	104976.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

174.80	8867.0
175.80	100320.0
176.80	6293.0
178.00	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.80	959.0
36.80	5552.0
37.90	4921.0
38.90	2647.0
40.10	533.0
42.80	165.0
43.90	1314.0
44.80	1133.0
45.80	379.0
46.80	1826.0
47.80	844.0
48.90	5628.0
49.90	24992.0
50.90	8079.0
51.90	595.0
52.80	297.0
53.70	368.0
54.80	333.0
55.80	1764.0
56.90	4068.0
57.80	218.0
59.80	1691.0
60.90	7344.0
61.90	7135.0
62.90	6928.0
63.80	1509.0
64.90	1927.0
65.70	155.0
66.80	369.0
67.80	14474.0
68.90	13655.0
69.90	1622.0
71.90	732.0
72.90	6885.0
73.90	24624.0
74.90	72272.0
75.90	6924.0
76.70	785.0
77.80	478.0
78.80	6397.0
79.80	1464.0
80.70	7067.0
81.80	1243.0
82.60	198.0
85.70	222.0
86.80	6895.0
87.90	5211.0
90.80	699.0
91.90	4862.0
92.80	5990.0
93.90	16174.0
94.90	143040.0
95.80	9393.0
96.90	382.0
102.60	110.0
103.80	576.0
104.70	178.0
105.70	713.0
106.70	224.0
107.80	307.0
110.10	123.0
111.70	140.0
112.60	203.0
114.60	230.0
115.70	565.0
116.80	1394.0
117.60	531.0
118.70	1137.0
125.70	109.0
127.70	550.0
128.60	150.0
129.80	644.0
130.60	143.0
134.70	282.0
136.70	377.0
140.80	1644.0
141.90	182.0
142.80	3167.0
143.60	207.0
144.80	1532.0
146.00	278.0
147.70	326.0
148.70	143.0
149.50	102.0
152.80	158.0
154.60	344.0
156.70	230.0
158.70	229.0
160.70	245.0
170.80	821.0
171.80	2171.0
172.90	2091.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

173.80	112752.0
174.80	9076.0
175.80	107672.0
176.80	6666.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.80	835.0
36.80	5358.0
37.80	4702.0
38.90	2346.0
40.10	474.0
42.80	140.0
43.90	1448.0
44.80	1025.0
45.80	333.0
46.90	1839.0
47.80	688.0
48.90	5131.0
49.90	22896.0
50.90	7232.0
51.90	573.0
52.80	281.0
53.70	330.0
54.80	308.0
55.90	1664.0
56.80	3854.0
57.80	163.0
59.10	106.0
59.80	1611.0
60.90	6984.0
61.90	6736.0
62.90	6761.0
63.80	1524.0
64.90	2070.0
65.70	174.0
66.80	368.0
67.80	13528.0
68.80	12850.0
69.90	1229.0
71.90	693.0
72.90	6258.0
73.90	22744.0
74.90	68640.0
75.90	6307.0
76.70	679.0
77.70	462.0
78.80	6274.0
79.80	1411.0
80.80	6781.0
81.80	1209.0
82.70	185.0
85.80	255.0
86.80	6503.0
87.80	5016.0
90.80	601.0
91.90	4472.0
92.80	5308.0
93.90	15071.0
94.90	134912.0
95.90	8631.0
96.90	293.0
103.80	579.0
104.90	233.0
105.70	626.0
106.70	150.0
107.80	338.0
110.00	113.0
111.60	141.0
112.60	149.0
114.60	213.0
115.80	667.0
116.80	1295.0
117.60	494.0
118.70	972.0
127.80	446.0
128.70	152.0
129.70	565.0
130.70	154.0
134.70	281.0
135.80	129.0
136.70	403.0
139.80	138.0
140.80	1491.0
141.70	136.0
142.80	3024.0
143.60	181.0
144.80	1334.0
145.90	326.0
147.70	358.0
152.80	156.0
154.60	382.0
156.70	191.0
157.00	202.0
158.70	245.0
160.80	284.0
170.80	728.0
171.80	2451.0
173.80	108824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

174.80	8214.0
175.80	103584.0
176.80	6415.0
177.80	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282