

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071519\
 Data File : VV011887.D
 Acq On : 15 Jul 2019 15:44
 Operator : SY/MD
 Sample : K3785-10
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XL8

Quant Time: Jul 16 04:24:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 16 03:56:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	178939	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	173892	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	79299	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	57425	4.27	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.40%
7) Chloroethane-d5	1.58	69	49594	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.20%
11) 1,1-Dichloroethene-d2	2.13	63	78357	3.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.00%
20) 2-Butanone-d5	3.94	46	142126	50.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.72%
24) Chloroform-d	4.40	84	110681	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.08	65	60278	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.10	84	225547	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.12	67	69179	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.36	98	195509	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	7.66	79	22650	4.19	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.80%
46) 2-Hexanone-d5	8.13	63	86594	40.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.54%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	33391	3.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	73.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	69909	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds				Ovalue
13) Acetone	2.20	43	13449	7.772 ug/L 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071519\
Data File : VV011887.D
Acq On : 15 Jul 2019 15:44
Operator : SY/MD
Sample : K3785-10
Misc : 25ML/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XL8

Quant Time: Jul 16 04:24:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 16 03:56:26 2019
Response via : Initial Calibration

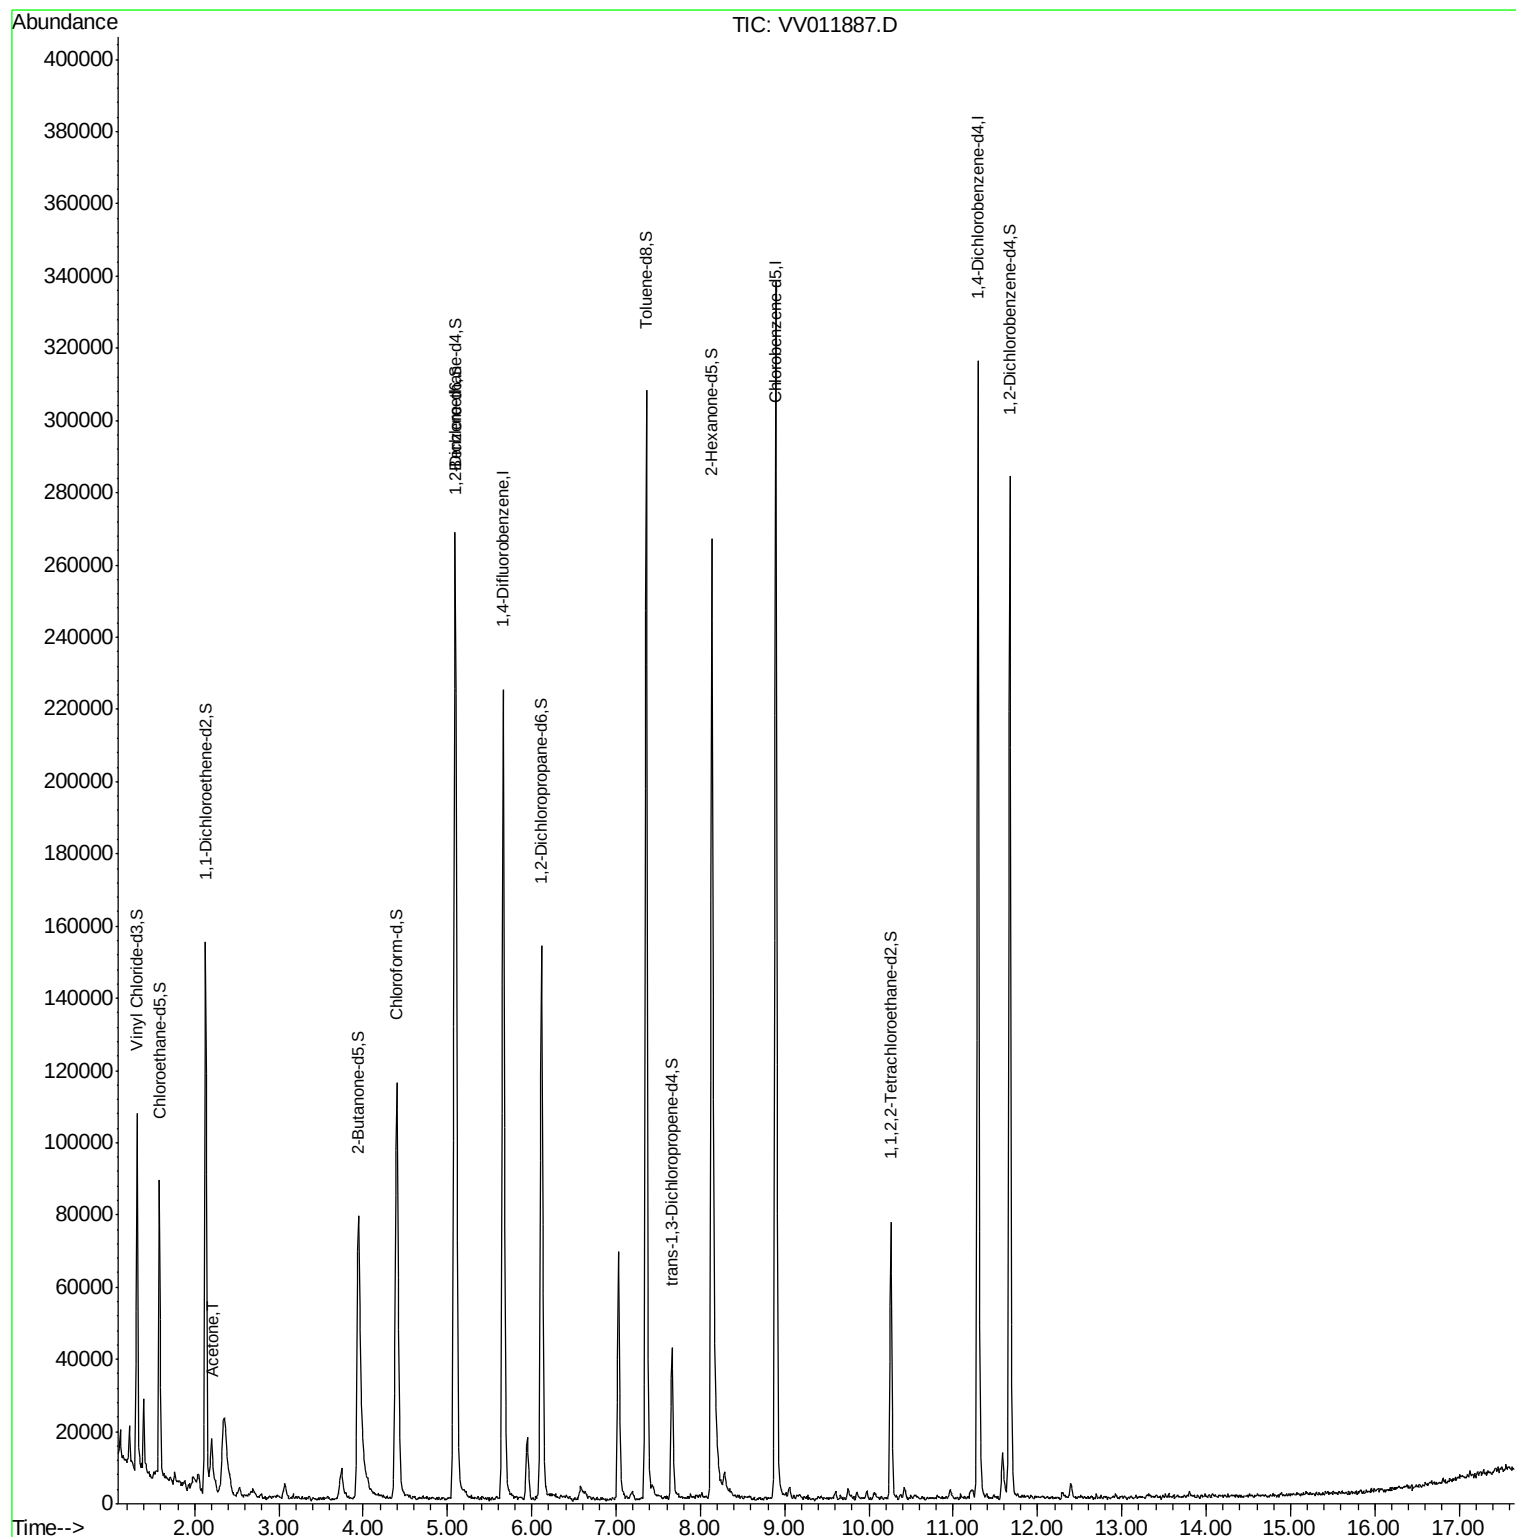

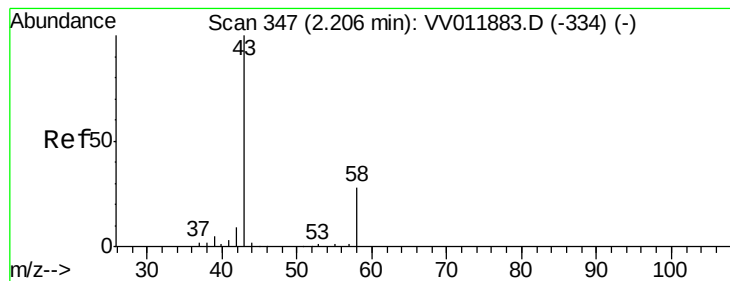

#13

Acetone

Concen: 7.772 ug/L

RT: 2.20 min Scan# 346

Delta R.T. -0.00 min

Lab File: VV011887.D

Acq: 15 Jul 2019 15:44

Instrument :
MSVOA_V
ClientSampleId :
C0XL8

Tot Ion: 43 Resp: 13449

Ion Ratio Lower Upper

43 100

58 30.1 0.0 58.4

