

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071519\
 Data File : VV011888.D
 Acq On : 15 Jul 2019 17:25
 Operator : SY/MD
 Sample : K3785-11
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 16 04:39:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 16 03:56:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	180585	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	178552	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	78010	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	55666	4.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.00%
7) Chloroethane-d5	1.58	69	48393	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.13	63	85396	3.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.80%
20) 2-Butanone-d5	3.95	46	144464	50.72	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.44%
24) Chloroform-d	4.40	84	109086	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.08	65	59414	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.10	84	221411	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
36) 1,2-Dichloropropane-d6	6.12	67	68419	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.20%
41) Toluene-d8	7.36	98	189241	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	7.66	79	21487	3.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.40%
46) 2-Hexanone-d5	8.14	63	92339	42.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.68%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	36147	3.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	68001	4.71	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.20%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	6622	0.648 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071519\
Data File : VV011888.D
Acq On : 15 Jul 2019 17:25
Operator : SY/MD
Sample : K3785-11
Misc : 25ML/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 16 04:39:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 16 03:56:26 2019
Response via : Initial Calibration

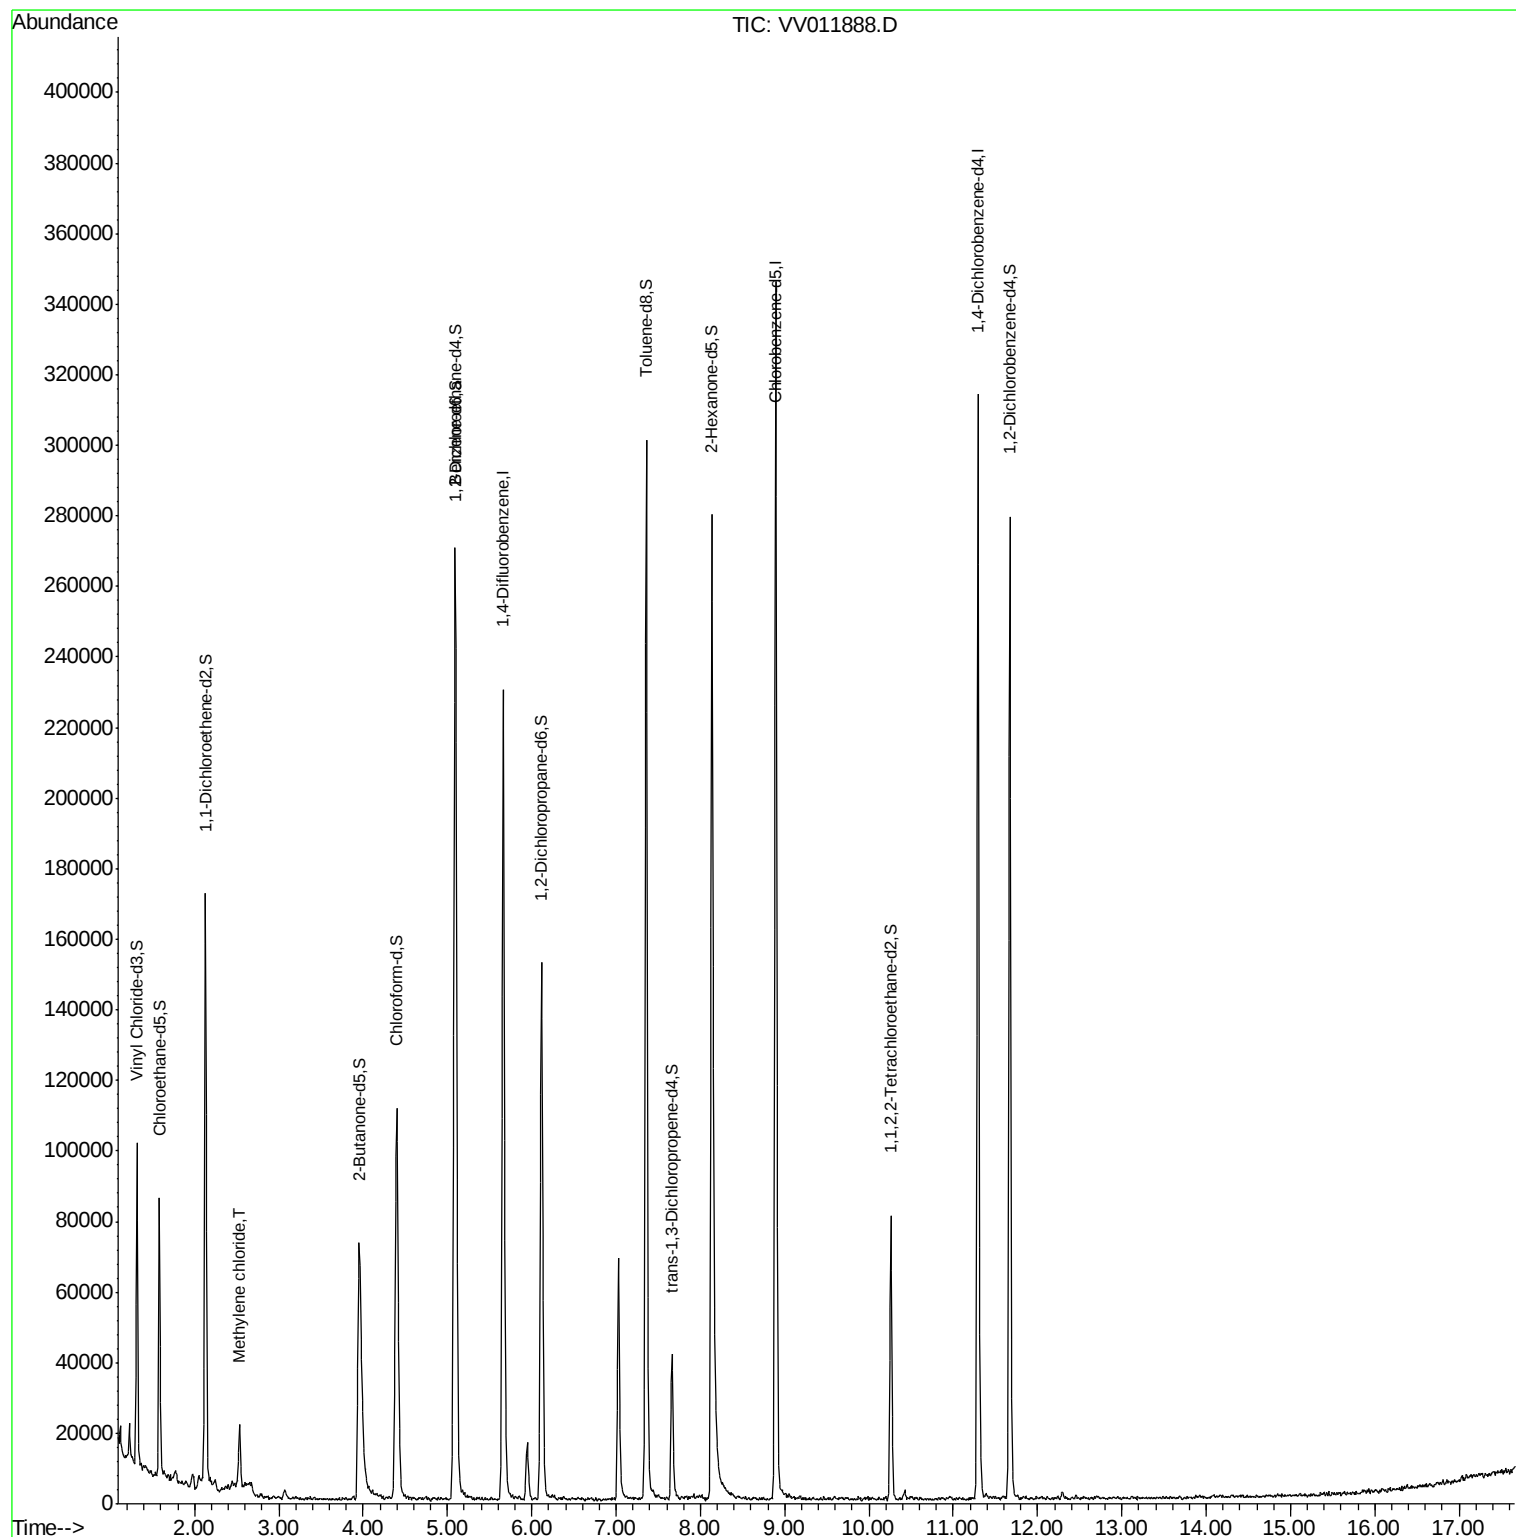

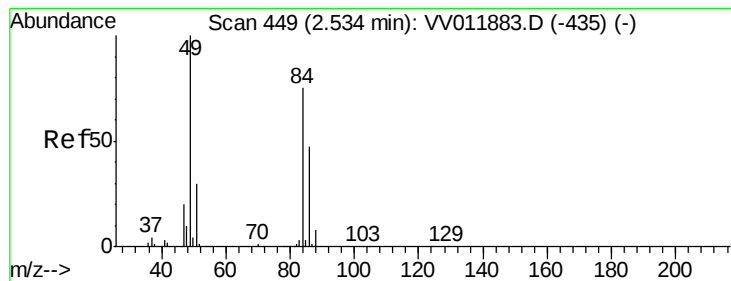

#16
Methylene chloride
Concen: 0.648 ug/L
RT: 2.53 min Scan# 449
Delta R.T. 0.00 min
Lab File: VV011888.D
Acq: 15 Jul 2019 17:25

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion: 84 Resp: 6622

Ion	Ratio	Lower	Upper
84	100		
86	60.6	43.9	81.5
49	137.8	92.6	172.0

