


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071519\
Data File : VV011882.D
Acq On : 15 Jul 2019 10:00
Operator : SY/MD
Sample : BFB32
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB32

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jul 16 03:56:26 2019

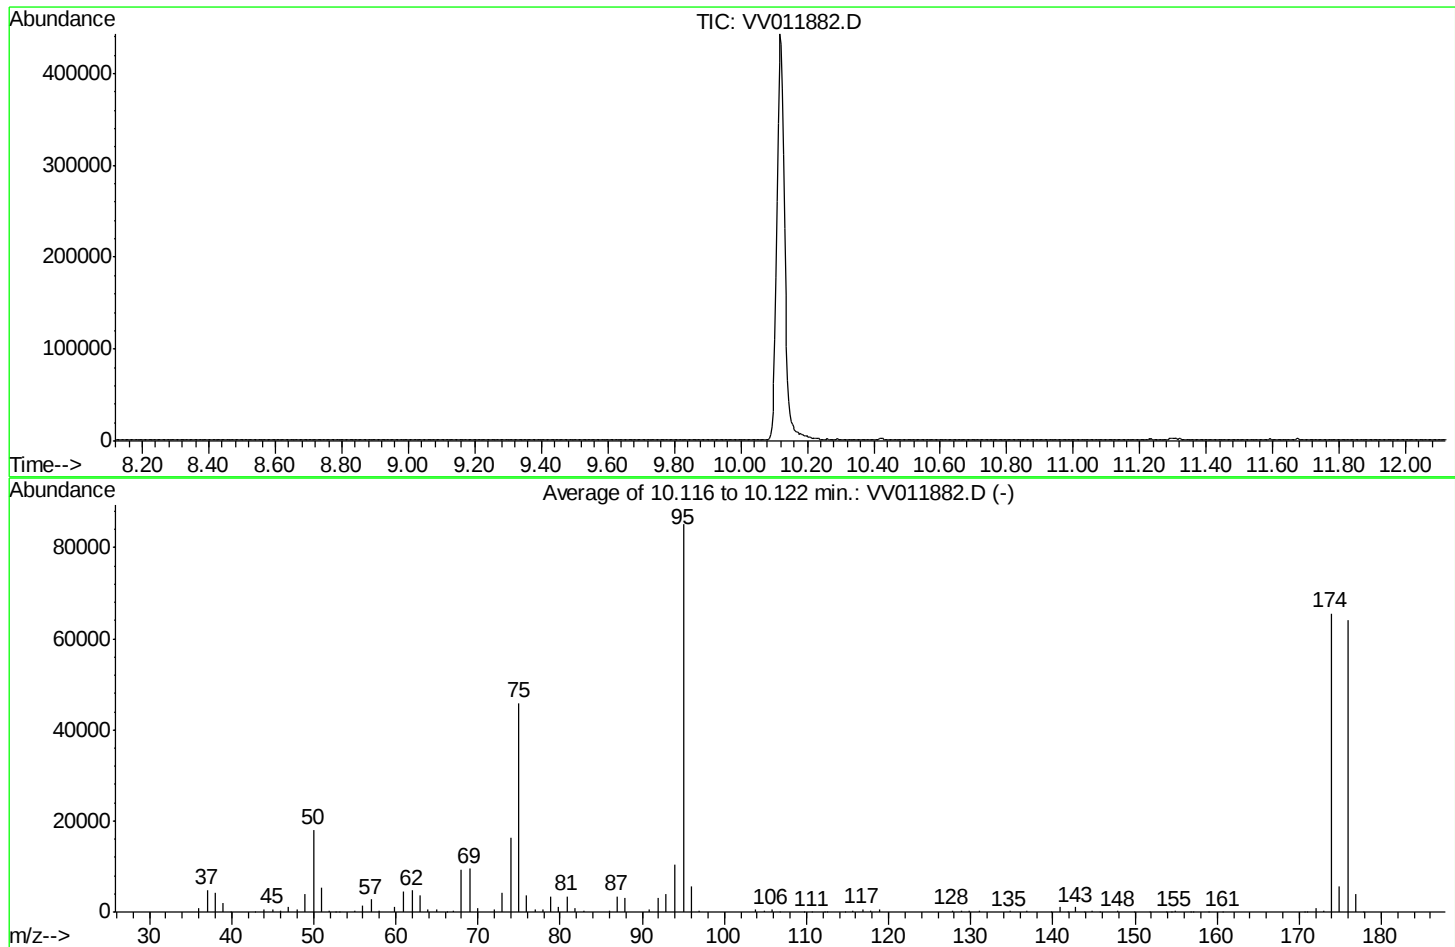

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	18114	PASS
75	95	30	80	53.8	45829	PASS
95	95	100	100	100.0	85149	PASS
96	95	5	9	6.6	5640	PASS
173	174	0.00	2	0.5	335	PASS
174	95	50	120	77.0	65592	PASS
175	174	5	9	8.4	5504	PASS
176	174	95	101	97.9	64192	PASS
177	176	5	9	6.0	3850	PASS

Scan 2794 (10.074 min): VV011882.D
BFB32

m/z	Abundance
39.90	321.0
40.80	105.0
41.10	101.0
43.80	481.0
47.70	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
35.90	794.0
37.00	4712.0
38.00	4319.0
39.00	1866.0
39.90	441.0
42.80	162.0
44.00	1002.0
45.00	686.0
46.00	195.0
46.80	1083.0
47.90	642.0
49.00	3856.0
50.00	17696.0
51.00	5331.0
52.00	353.0
52.70	148.0
55.00	218.0
55.90	1390.0
56.90	2687.0
57.90	178.0
59.90	972.0
61.00	4618.0
62.00	4527.0
63.00	3523.0
63.90	576.0
64.90	517.0
66.10	128.0
67.00	258.0
68.00	9015.0
69.00	9327.0
69.90	825.0
72.00	542.0
72.90	3965.0
74.00	15817.0
75.00	44272.0
75.90	3608.0
76.90	498.0
77.80	442.0
78.90	3080.0
79.80	1041.0
80.80	3386.0
81.90	782.0
82.90	206.0
86.10	161.0
86.90	3476.0
87.90	3040.0
90.90	449.0
92.00	2909.0
92.90	3727.0
94.00	10000.0
95.00	82456.0
96.00	5468.0
96.90	210.0
103.80	386.0
104.90	181.0
105.80	427.0
109.70	103.0
110.70	128.0
112.20	104.0
115.70	342.0
116.80	664.0
117.80	377.0
118.80	605.0
127.80	292.0
128.90	191.0
129.80	367.0
131.00	174.0
134.80	176.0
136.80	135.0
140.90	1071.0
142.80	993.0
144.80	235.0
145.70	139.0
147.80	237.0
149.80	131.0
154.50	125.0
155.00	139.0
157.10	155.0
158.90	108.0
160.80	129.0
170.60	168.0
172.00	890.0
173.00	1005.0
173.90	61896.0
174.90	5277.0
175.90	60312.0
176.90	3447.0
177.80	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
35.90	911.0
37.00	5097.0
38.00	4216.0
39.00	2029.0
39.80	480.0
40.80	103.0
42.80	158.0
44.00	1003.0
45.00	689.0
46.00	214.0
46.80	1084.0
48.00	736.0
48.90	4139.0
50.00	18720.0
51.00	5603.0
51.90	385.0
52.70	123.0
53.10	103.0
55.00	218.0
55.90	1449.0
57.00	2798.0
58.00	236.0
59.90	1107.0
60.90	4790.0
62.00	4861.0
63.00	3731.0
63.90	601.0
64.90	599.0
66.20	107.0
66.90	307.0
68.00	9756.0
69.00	9835.0
69.90	872.0
72.00	549.0
72.90	4310.0
74.00	16760.0
75.00	47456.0
76.00	3840.0
77.00	540.0
77.90	467.0
78.90	3375.0
79.90	1089.0
80.80	3423.0
81.90	805.0
83.00	191.0
86.00	158.0
86.90	3611.0
87.90	3116.0
90.90	490.0
92.00	3098.0
92.90	3933.0
94.00	10637.0
95.00	88136.0
96.00	5898.0
96.90	192.0
103.80	445.0
104.90	197.0
105.80	479.0
106.70	118.0
109.70	106.0
110.70	120.0
112.30	112.0
115.70	368.0
116.80	691.0
117.80	439.0
118.90	651.0
127.80	359.0
128.80	182.0
129.80	334.0
131.00	201.0
134.80	204.0
136.80	148.0
139.80	113.0
140.80	1126.0
141.80	142.0
142.80	1140.0
143.90	100.0
144.80	251.0
145.70	145.0
147.90	263.0
149.90	110.0
154.90	161.0
156.80	132.0
158.90	119.0
160.80	152.0
172.00	981.0
173.90	67624.0
174.90	5713.0
175.90	66400.0
176.90	3908.0
177.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
35.90	970.0
37.00	4861.0
38.00	4041.0
39.00	1970.0
39.80	466.0
40.90	123.0
42.90	118.0
43.90	995.0
44.90	714.0
46.00	216.0
46.90	971.0
48.00	725.0
48.90	4000.0
50.00	17928.0
51.00	5472.0
51.90	360.0
53.10	106.0
54.80	234.0
55.00	224.0
55.90	1424.0
57.00	2705.0
58.00	275.0
59.90	1067.0
61.00	4353.0
61.90	4750.0
63.00	3569.0
63.90	569.0
64.90	654.0
66.30	112.0
66.90	328.0
68.00	9441.0
69.00	9362.0
69.90	792.0
72.00	532.0
72.90	4305.0
74.00	16045.0
75.00	45760.0
76.00	3710.0
77.00	517.0
77.80	413.0
78.90	3358.0
79.80	1053.0
80.90	3371.0
81.80	835.0
83.00	164.0
85.90	149.0
86.90	3321.0
87.90	3059.0
90.90	493.0
91.90	2926.0
92.90	3841.0
94.00	10707.0
95.00	84856.0
96.00	5556.0
97.00	161.0
103.80	466.0
104.80	176.0
105.80	475.0
106.80	118.0
109.70	103.0
112.50	104.0
114.70	130.0
115.70	334.0
116.80	635.0
117.80	458.0
118.80	609.0
127.70	403.0
128.80	160.0
129.70	291.0
131.00	192.0
134.80	226.0
136.80	179.0
139.90	122.0
140.80	1034.0
141.70	194.0
142.80	1147.0
143.90	136.0
144.90	256.0
145.80	159.0
148.00	265.0
151.80	102.0
153.80	101.0
154.80	183.0
156.70	173.0
158.90	126.0
160.70	171.0
171.00	198.0
172.00	870.0
173.90	67256.0
174.90	5523.0
175.90	65864.0
176.90	4195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32