


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071520\
 Data File : VV017498.D
 Acq On : 15 Jul 2020 08:41
 Operator : SY/MD
 Sample : BFB50
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB50

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 16 01:29:31 2020

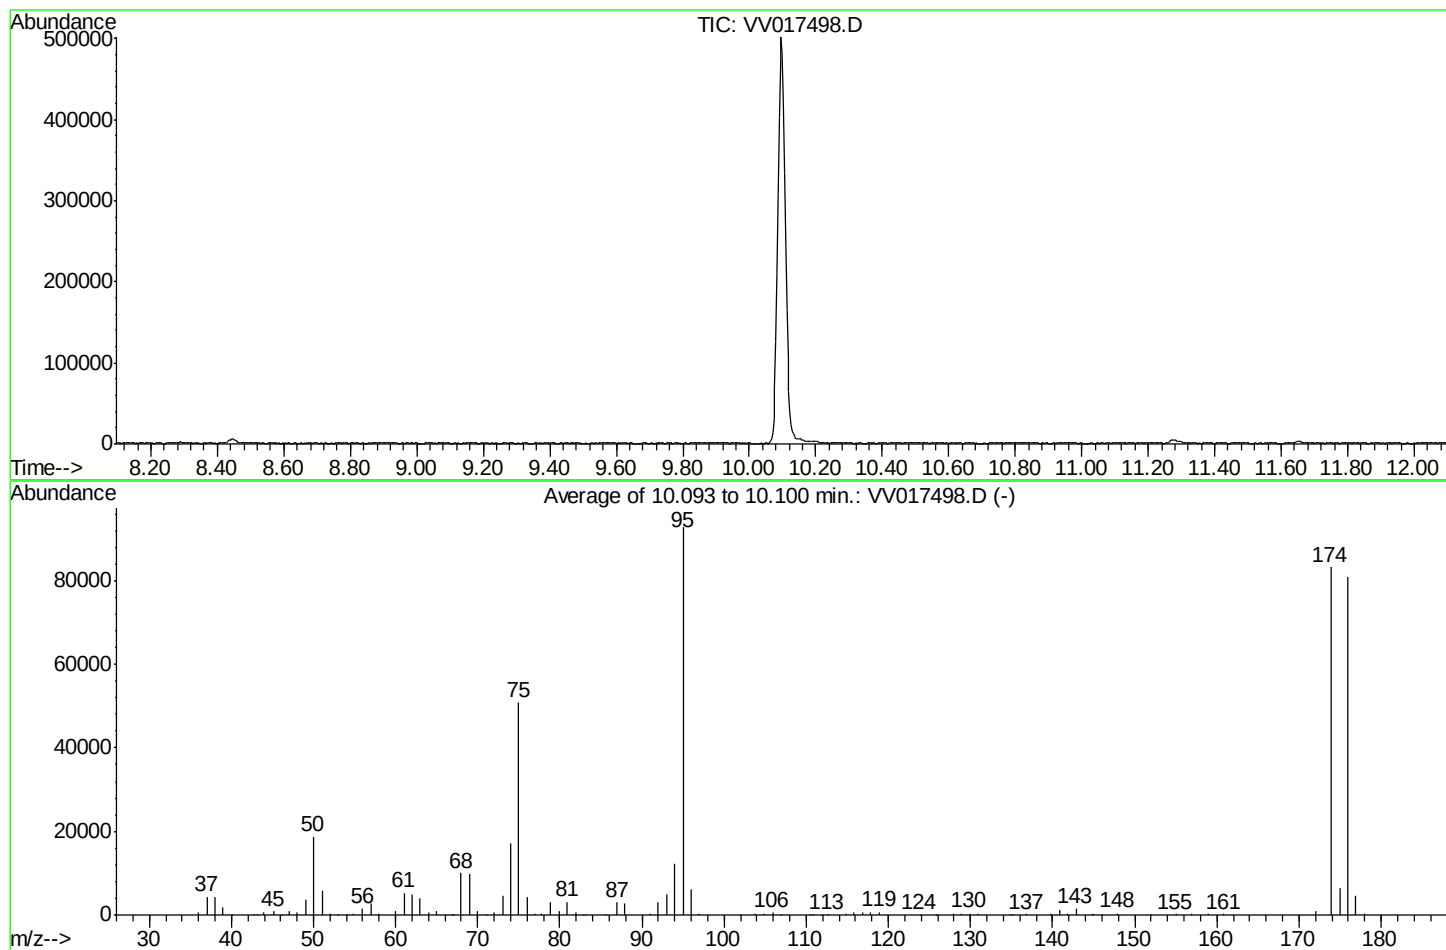

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	18813	PASS
75	95	30	80	54.8	50837	PASS
95	95	100	100	100.0	92765	PASS
96	95	5	9	6.6	6088	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.8	83304	PASS
175	174	5	9	7.6	6294	PASS
176	174	95	101	97.0	80794	PASS
177	176	5	9	5.9	4730	PASS

m/z	Abundance
36.00	761.0
37.00	4395.0
38.00	4568.0
39.00	1765.0
40.00	294.0
44.00	759.0
45.10	926.0
46.00	167.0
47.10	867.0
48.00	757.0
49.00	3814.0
50.00	18184.0
51.10	5712.0
52.00	353.0
53.00	149.0
54.90	468.0
55.90	1469.0
57.00	2808.0
57.80	250.0
59.90	842.0
61.00	5060.0
62.00	4605.0
63.00	3900.0
63.90	659.0
65.00	944.0
66.00	183.0
66.80	254.0
68.00	9690.0
69.00	9714.0
70.00	812.0
72.00	599.0
73.00	4567.0
74.00	17424.0
75.00	50016.0
76.10	4541.0
77.00	443.0
77.80	284.0
78.90	2850.0
79.90	1007.0
80.90	3116.0
81.90	713.0
82.70	105.0
85.60	104.0
87.00	3065.0
87.90	2744.0
90.90	439.0
92.00	3102.0
93.00	4844.0
94.00	12129.0
95.00	90088.0
96.00	6114.0
97.00	244.0
103.80	392.0
104.90	225.0
105.80	506.0
106.80	114.0
110.50	102.0
112.70	127.0
114.90	144.0
115.80	472.0
116.90	764.0
117.90	464.0
119.00	794.0
123.80	112.0
125.70	104.0
128.00	417.0
128.80	202.0
129.90	465.0
131.00	235.0
134.80	188.0
136.80	194.0
139.70	167.0
140.90	1269.0
141.80	184.0
142.90	1298.0
144.80	307.0
146.10	126.0
147.90	327.0
155.00	223.0
156.80	164.0
158.90	198.0
160.80	163.0
172.00	1105.0
173.90	80984.0
175.00	6106.0
176.00	76736.0
177.00	4628.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	796.0
37.00	4558.0
38.00	4487.0
39.00	1785.0
40.00	283.0
42.80	108.0
44.00	839.0
45.10	907.0
46.00	169.0
47.10	1018.0
47.90	768.0
49.00	3893.0
50.00	19416.0
51.00	6117.0
52.00	314.0
53.00	160.0
54.90	457.0
56.00	1545.0
57.00	2914.0
57.90	231.0
59.90	912.0
61.00	5509.0
62.00	5016.0
63.00	4037.0
64.00	618.0
65.00	1040.0
66.00	146.0
68.00	10398.0
69.00	10058.0
70.00	795.0
71.00	111.0
71.90	617.0
73.00	4781.0
74.00	17664.0
75.00	52680.0
76.10	4514.0
77.00	450.0
77.80	306.0
78.90	3056.0
80.00	971.0
80.90	3300.0
81.90	679.0
83.00	110.0
85.50	131.0
87.00	3086.0
87.90	2826.0
91.00	466.0
92.00	3333.0
93.00	5215.0
94.00	12852.0
95.00	95944.0
96.00	6307.0
96.90	217.0
103.90	484.0
104.80	228.0
105.90	538.0
106.80	145.0
111.90	126.0
112.60	145.0
114.80	175.0
115.80	489.0
116.90	713.0
117.80	510.0
118.90	793.0
123.90	123.0
125.90	106.0
127.90	463.0
128.80	192.0
129.90	496.0
130.90	265.0
134.90	164.0
136.80	182.0
139.70	177.0
140.90	1335.0
141.80	189.0
142.90	1461.0
145.00	322.0
146.00	115.0
147.90	321.0
151.90	133.0
155.00	223.0
156.90	189.0
158.90	214.0
160.90	240.0
172.00	1095.0
173.90	86088.0
175.00	6453.0
176.00	83432.0
176.90	4876.0
177.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	721.0
37.10	4246.0
38.00	4113.0
39.00	1608.0
40.00	254.0
42.70	133.0
43.10	106.0
44.00	881.0
45.10	796.0
46.10	149.0
47.10	1129.0
47.90	722.0
49.00	3760.0
50.00	18840.0
51.00	5909.0
52.10	275.0
53.00	153.0
54.00	114.0
54.90	373.0
56.00	1474.0
57.00	2631.0
58.00	226.0
59.90	963.0
61.00	5390.0
62.00	4822.0
63.00	3795.0
64.00	450.0
65.00	930.0
67.00	367.0
68.00	10175.0
69.00	9742.0
70.00	770.0
71.00	123.0
71.90	619.0
73.00	4559.0
74.00	16302.0
75.00	49816.0
76.10	4140.0
77.00	396.0
77.80	287.0
78.90	2998.0
80.00	962.0
80.90	3232.0
81.90	678.0
83.00	149.0
85.50	107.0
87.00	2696.0
87.90	2589.0
91.00	440.0
92.00	3097.0
93.00	5062.0
94.00	12211.0
95.00	92264.0
96.00	5845.0
96.90	194.0
101.90	101.0
103.90	533.0
104.70	172.0
106.00	527.0
106.90	170.0
110.60	105.0
110.80	105.0
111.90	145.0
112.60	116.0
114.80	237.0
115.80	464.0
116.90	600.0
117.80	475.0
118.90	714.0
123.90	117.0
125.90	106.0
127.80	485.0
128.90	192.0
130.00	450.0
130.90	247.0
134.70	138.0
135.10	150.0
136.90	178.0
139.80	166.0
141.00	1292.0
141.80	183.0
142.90	1482.0
145.00	353.0
145.90	153.0
147.90	318.0
151.90	147.0
155.00	232.0
156.90	210.0
158.90	174.0
160.90	244.0
172.00	1009.0
173.90	82840.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

175.00	6324.0
176.00	82216.0
176.90	4688.0
178.00	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

Scan 2788 (10.055 min): VV017498.D
BFB50

m/z	Abundance
40.00	185.0
43.90	178.0
46.30	177.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50