

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071521\
 Data File : VW021663.D
 Acq On : 15 Jul 2021 11:12
 Operator : SY/MD
 Sample : M3033-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :

Quant Time: Jul 16 01:07:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 16 01:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	546652	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	510773	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	263961	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	101890	29.460	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	58.920%#		
7) Chloroethane-d5	1.561	69	84071	29.741	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	59.480%#		
11) 1,1-Dichloroethene-d2	2.105	63	140222	22.159	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	44.320%#		
21) 2-Butanone-d5	3.867	46	172943	58.548	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	58.550%		
24) Chloroform-d	4.342	84	214800	29.691	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	59.380%#		
26) 1,2-Dichloroethane-d4	5.027	65	135724	31.839	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	63.680%#		
32) Benzene-d6	5.047	84	445403	31.057	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	62.120%#		
36) 1,2-Dichloropropane-d6	6.066	67	141865	31.363	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	62.720%#		
41) Toluene-d8	7.313	98	412763	31.121	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	62.240%#		
43) trans-1,3-Dichloroprop...	7.622	79	68413	30.405	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	60.800%		
47) 2-Hexanone-d5	8.085	63	111338	53.064	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	53.060%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	185766	30.482	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	60.960%#		
66) 1,2-Dichlorobenzene-d4	11.625	152	166314	31.604	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	63.200%#		
Target Compounds						
					Qvalue	
13) Acetone	2.159	43	8231	3.371	ug/L #	100
61) 1,2,3-Trichloropropane	11.249	75	28714	5.627	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
 Data File : VV021663.D
 Acq On : 15 Jul 2021 11:12
 Operator : SY/MD
 Sample : M3033-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :

Quant Time: Jul 16 01:07:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 16 01:06:31 2021
 Response via : Initial Calibration




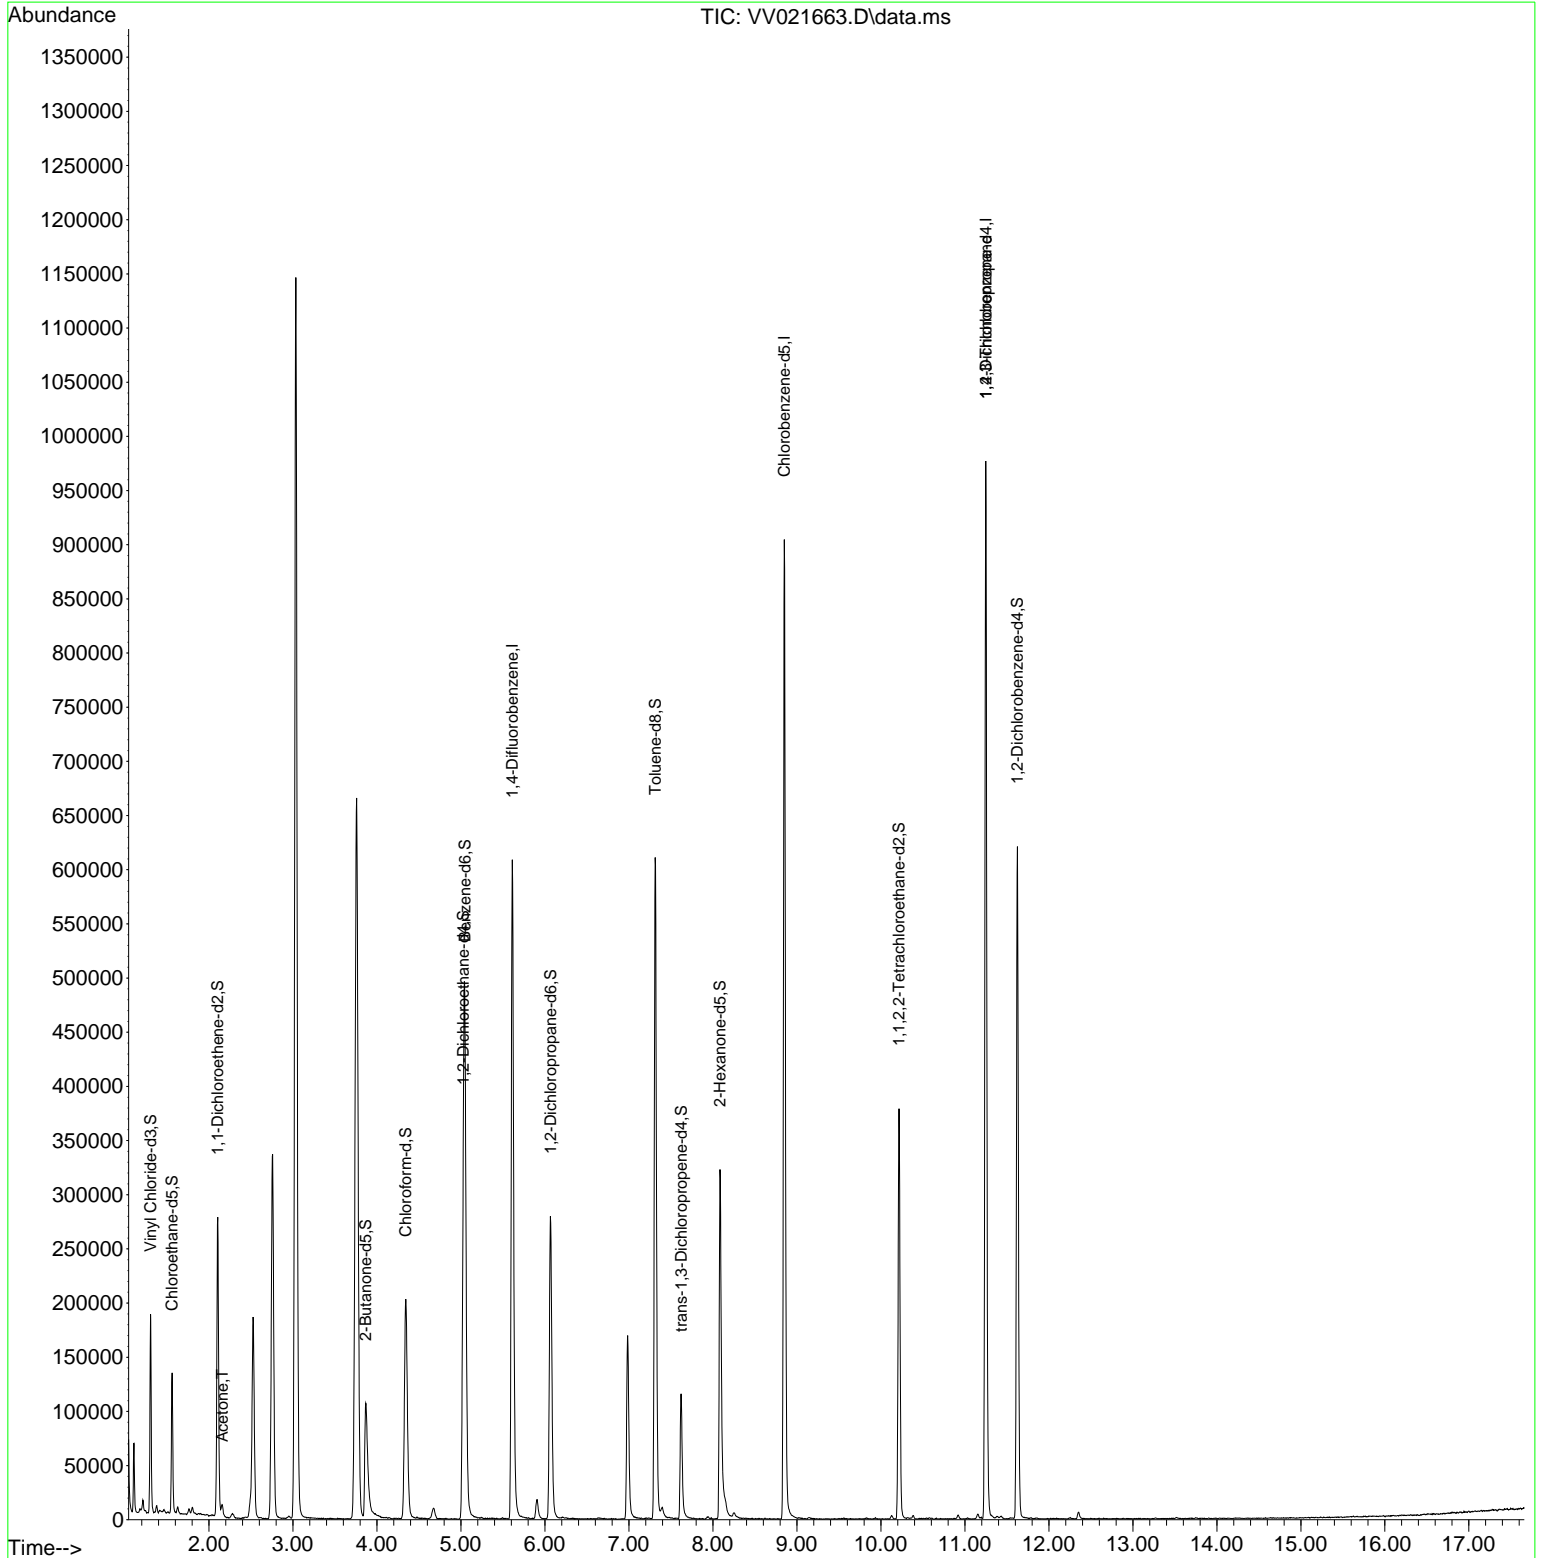


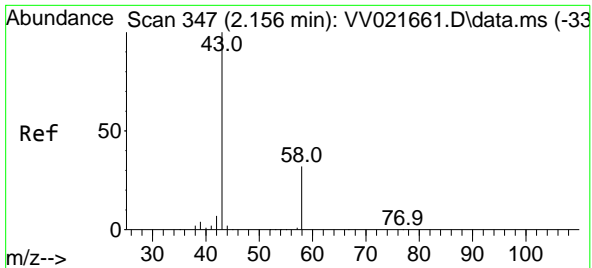

#13
 Acetone
 Concen: 3.371 ug/L
 RT: 2.159 min Scan# 348
 Delta R.T. 0.003 min
 Lab File: VV021663.D
 Acq: 15 Jul 2021 11:12

Instrument :
 MSVOA_V
 ClientSampled :

Tgt Ion: 43 Resp: 8231
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 0.0#

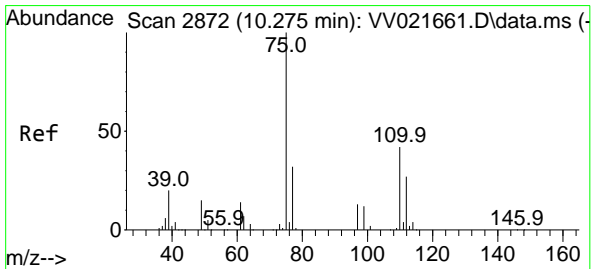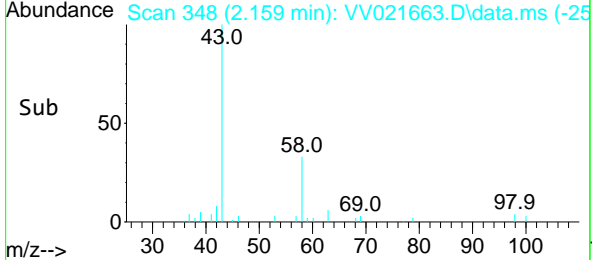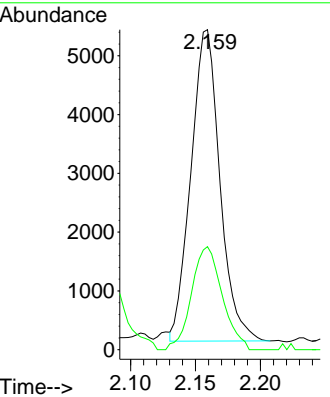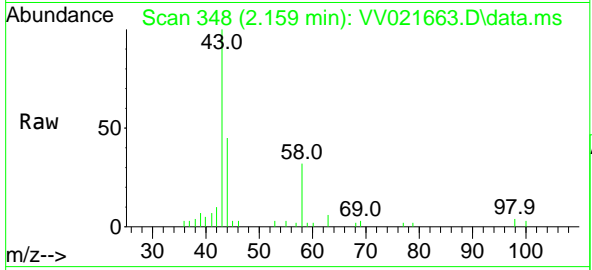

#61
 1,2,3-Trichloropropane
 Concen: 5.627 ug/L
 RT: 11.249 min Scan# 3175
 Delta R.T. 0.974 min
 Lab File: VV021663.D
 Acq: 15 Jul 2021 11:12

Tgt Ion: 75 Resp: 28714
 Ion Ratio Lower Upper
 75 100
 77 32.2 25.8 38.8
 110 3.2 33.0 49.6#

