

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
 Data File : VV021671.D
 Acq On : 15 Jul 2021 15:42
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M

Title : VOC Analysis

Signal : TIC: VV021671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	175781	184827	12.22%	1.578%
2	1.548	152	158	171	rVB	141558	167514	11.08%	1.430%
3	2.101	320	330	349	rBV	304235	449274	29.71%	3.836%
4	2.503	446	455	469	rVB2	9680	16558	1.09%	0.141%
5	2.706	516	518	521	rVB2	419	233	0.02%	0.002%
6	2.725	521	524	526	rBV	319	196	0.01%	0.002%
7	2.761	526	535	536	rBV3	2270	2360	0.16%	0.020%
8	2.883	571	573	577	rBV2	463	260	0.02%	0.002%
9	3.082	632	635	638	rBV2	304	228	0.02%	0.002%
10	3.095	638	639	650	rVB4	497	677	0.04%	0.006%
11	3.140	650	653	657	rVB2	356	198	0.01%	0.002%
12	3.172	657	663	667	rBV3	333	401	0.03%	0.003%
13	3.252	686	688	692	rVB2	380	306	0.02%	0.003%
14	3.317	703	708	712	rVB	451	400	0.03%	0.003%
15	3.343	712	716	720	rBV3	334	359	0.02%	0.003%
16	3.410	735	737	742	rVB2	303	227	0.02%	0.002%
17	3.539	772	777	780	rVV2	300	201	0.01%	0.002%
18	3.597	789	795	800	rBV2	456	658	0.04%	0.006%
19	3.642	805	809	813	rVB2	357	257	0.02%	0.002%
20	3.670	813	818	821	rBV	337	246	0.02%	0.002%
21	3.728	833	836	842	rVB2	616	476	0.03%	0.004%
22	3.754	842	844	848	rBV2	297	180	0.01%	0.002%
23	3.773	848	850	853	rVB2	347	211	0.01%	0.002%
24	3.799	853	858	859	rBV2	212	170	0.01%	0.001%
25	3.870	870	880	924	rBV	131716	351280	23.23%	2.999%
26	4.342	1009	1027	1053	rBV	236719	590202	39.03%	5.039%
27	4.674	1127	1130	1132	rBV2	553	294	0.02%	0.003%
28	4.805	1168	1171	1173	rBV	350	186	0.01%	0.002%
29	4.905	1198	1202	1204	rBV3	302	211	0.01%	0.002%
30	5.040	1224	1244	1284	rBV2	589884	1512189	100.00%	12.910%
31	5.297	1323	1324	1328	rBV	292	167	0.01%	0.001%
32	5.339	1334	1337	1340	rVB3	576	347	0.02%	0.003%
33	5.471	1377	1378	1382	rVB2	464	230	0.02%	0.002%
34	5.532	1394	1397	1401	rBV	417	243	0.02%	0.002%
35	5.613	1409	1422	1453	rBV	479310	967368	63.97%	8.259%
36	5.902	1500	1512	1530	rBV2	20093	44325	2.93%	0.378%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071521\
 Data File : VW021671.D
 Acq On : 15 Jul 2021 15:42
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

37	5.998	1538	1542	1545	rBV3	617	447	0.03%	0.004%
38	6.069	1550	1564	1594	rVV	332925	681319	45.06%	5.817%
39	6.297	1632	1635	1639	rVB2	595	356	0.02%	0.003%
40	6.352	1650	1652	1654	rVV	398	149	0.01%	0.001%
41	6.368	1654	1657	1661	rVB2	564	392	0.03%	0.003%
42	6.391	1661	1664	1668	rBV2	503	318	0.02%	0.003%
43	6.423	1671	1674	1675	rBV	268	142	0.01%	0.001%
44	6.445	1679	1681	1685	rVB2	406	198	0.01%	0.002%
45	6.471	1686	1689	1690	rBV	312	157	0.01%	0.001%
46	6.510	1698	1701	1703	rBV2	300	167	0.01%	0.001%
47	6.519	1703	1704	1707	rVV2	452	227	0.02%	0.002%
48	6.545	1710	1712	1715	rVB	426	211	0.01%	0.002%
49	6.629	1734	1738	1739	rBV3	612	394	0.03%	0.003%
50	6.744	1771	1774	1780	rVB4	594	500	0.03%	0.004%
51	6.773	1780	1783	1786	rBV2	411	253	0.02%	0.002%
52	6.844	1801	1805	1810	rBV	397	364	0.02%	0.003%
53	6.870	1812	1813	1815	rVV	418	191	0.01%	0.002%
54	6.985	1837	1849	1876	rBV	200195	362003	23.94%	3.090%
55	7.313	1939	1951	1970	rBV	713090	1236959	81.80%	10.560%
56	7.567	2029	2030	2035	rBV3	412	250	0.02%	0.002%
57	7.622	2037	2047	2073	rBV	134142	232611	15.38%	1.986%
58	7.825	2108	2110	2111	rBV	372	159	0.01%	0.001%
59	7.857	2118	2120	2123	rVB3	515	185	0.01%	0.002%
60	7.905	2130	2135	2136	rBV4	391	329	0.02%	0.003%
61	7.944	2141	2147	2150	rBV3	355	373	0.02%	0.003%
62	7.985	2157	2160	2162	rBV2	284	157	0.01%	0.001%
63	8.088	2182	2192	2227	rBV	408168	757905	50.12%	6.470%
64	8.519	2321	2326	2328	rBV3	415	417	0.03%	0.004%
65	8.661	2367	2370	2373	rVB3	344	172	0.01%	0.001%
66	8.696	2378	2381	2384	rBV2	516	364	0.02%	0.003%
67	8.715	2384	2387	2388	rBV	205	140	0.01%	0.001%
68	8.773	2402	2405	2407	rBV2	357	139	0.01%	0.001%
69	8.789	2408	2410	2413	rBV	329	172	0.01%	0.001%
70	8.850	2418	2429	2463	rBV	693167	1143253	75.60%	9.760%
71	9.352	2582	2585	2587	rBV2	356	180	0.01%	0.002%
72	9.481	2623	2625	2628	rVB2	268	159	0.01%	0.001%
73	9.554	2645	2648	2654	rBV3	525	563	0.04%	0.005%
74	9.583	2654	2657	2663	rVV2	339	355	0.02%	0.003%
75	9.722	2697	2700	2704	rBV	285	212	0.01%	0.002%
76	9.780	2716	2718	2724	rVB	303	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
 Data File : VV021671.D
 Acq On : 15 Jul 2021 15:42
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis

77	9.821	2728	2731	2735	rBV2	281	201	0.01%	0.002%
78	9.879	2744	2749	2755	rBV	211	299	0.02%	0.003%
79	10.034	2793	2797	2798	rBV3	409	210	0.01%	0.002%
80	10.104	2816	2819	2820	rVV2	460	231	0.02%	0.002%
81	10.127	2820	2826	2834	rVB3	2928	4337	0.29%	0.037%
82	10.217	2842	2854	2877	rBV	449923	706711	46.73%	6.033%
83	10.307	2879	2882	2885	rBV2	753	660	0.04%	0.006%
84	10.435	2919	2922	2924	rBV	343	201	0.01%	0.002%
85	10.455	2924	2928	2934	rVB2	458	441	0.03%	0.004%
86	10.484	2935	2937	2940	rBV	249	149	0.01%	0.001%
87	10.661	2986	2992	2997	rVB5	623	750	0.05%	0.006%
88	10.728	3011	3013	3016	rBV	268	150	0.01%	0.001%
89	10.831	3042	3045	3046	rBV2	276	174	0.01%	0.001%
90	10.841	3046	3048	3050	rVB	565	264	0.02%	0.002%
91	10.963	3083	3086	3088	rVB2	523	293	0.02%	0.003%
92	11.149	3136	3144	3151	rBV5	2129	3233	0.21%	0.028%
93	11.249	3163	3175	3195	rBV	729005	1141636	75.50%	9.746%
94	11.625	3279	3292	3314	rBV	716669	1128173	74.61%	9.631%
95	11.850	3356	3362	3364	rBV6	832	806	0.05%	0.007%
96	12.249	3484	3486	3492	rBV4	783	611	0.04%	0.005%
97	12.413	3535	3537	3541	rBV2	363	179	0.01%	0.002%
98	12.699	3623	3626	3631	rVV3	412	236	0.02%	0.002%
99	12.792	3653	3655	3657	rBV2	289	152	0.01%	0.001%
100	14.702	4245	4249	4253	rBV	10147	6870	0.45%	0.059%




Sum of corrected areas: 11713550

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
Data File : VV021671.D
Acq On : 15 Jul 2021 15:42
Operator : SY/MD
Sample : VIBLK202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

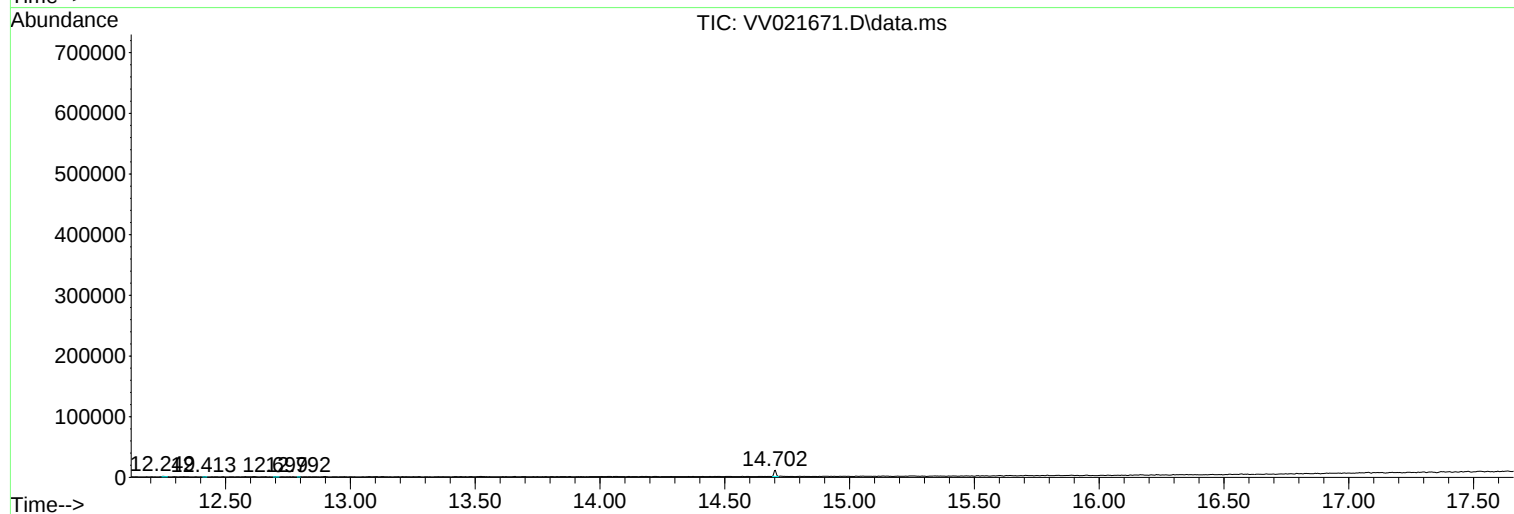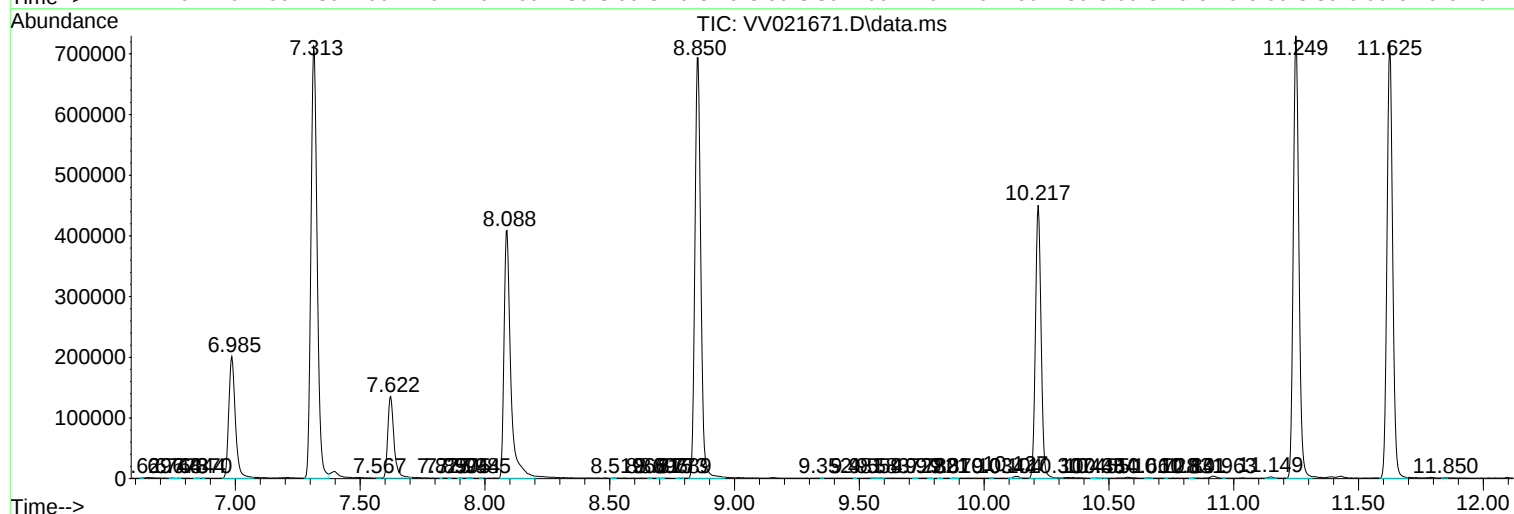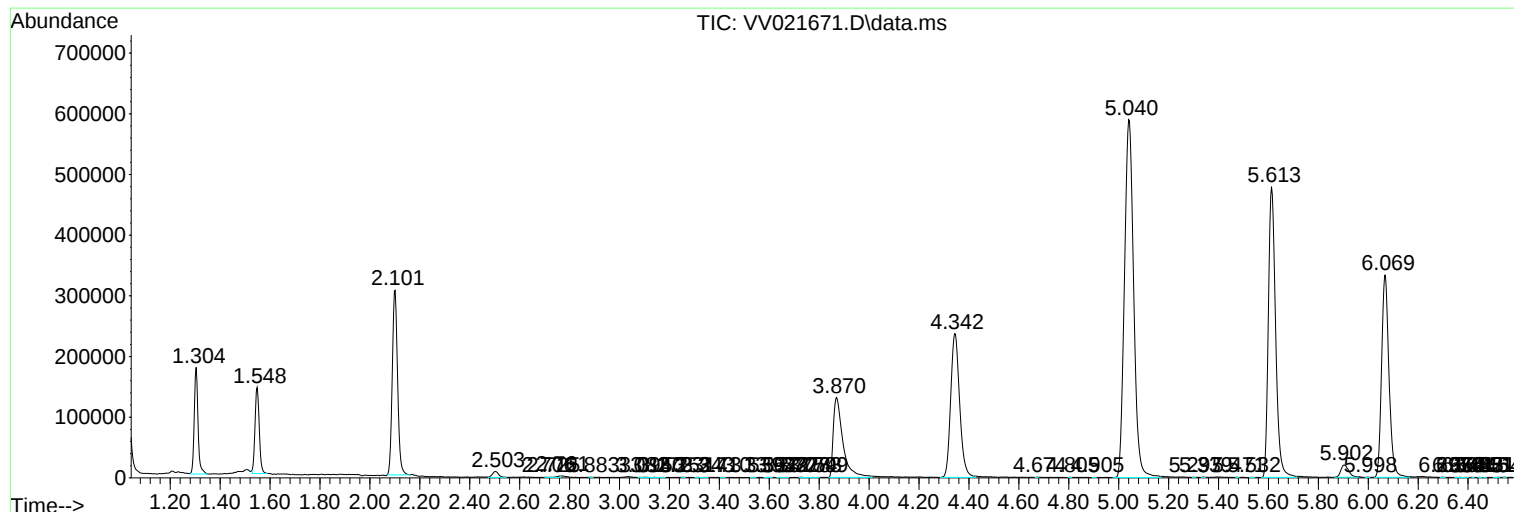

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
Data File : VV021671.D
Acq On : 15 Jul 2021 15:42
Operator : SY/MD
Sample : VIBLK202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
Data File : VV021671.D
Acq On : 15 Jul 2021 15:42
Operator : SY/MD
Sample : VIBLK202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
