
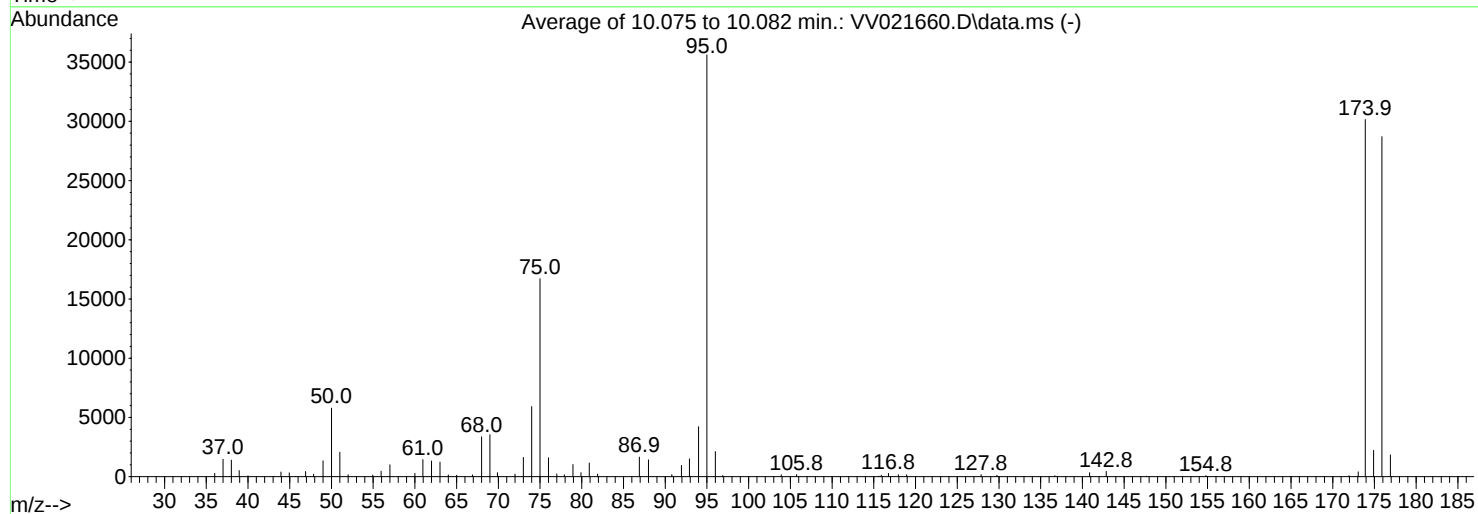


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071521\
 Data File : VV021660.D
 Acq On : 15 Jul 2021 08:49
 Operator : SY/MD
 Sample : BFB206
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB206

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM062921WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 16 01:06:31 2021

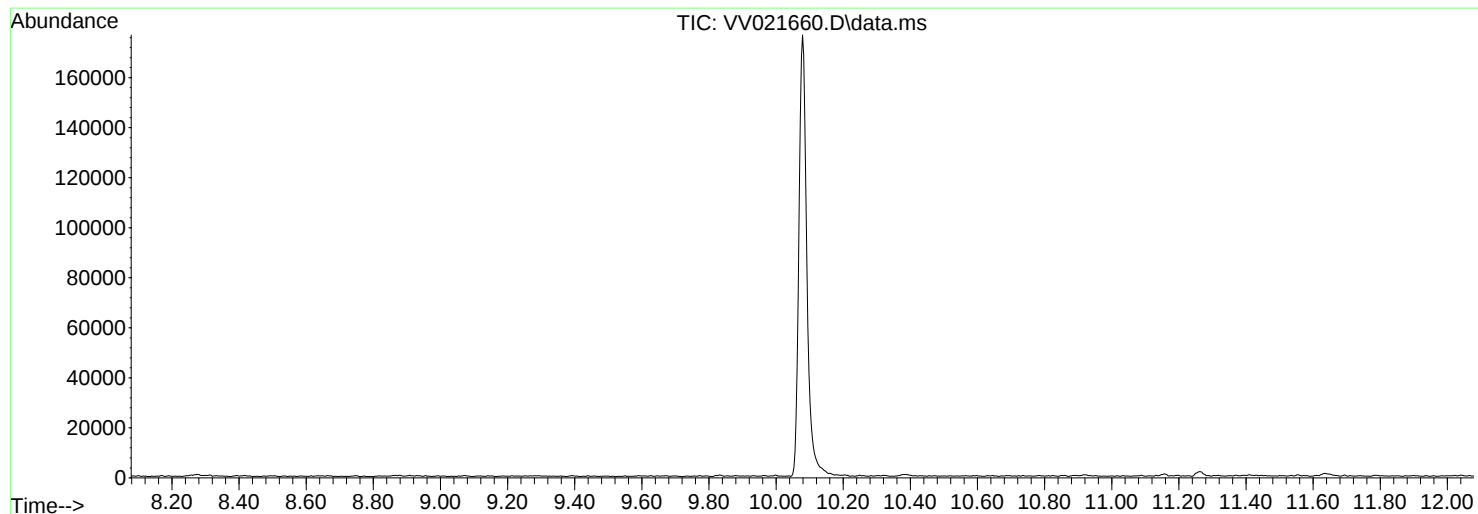

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	5779	PASS
75	95	30	80	46.9	16707	PASS
95	95	100	100	100.0	35616	PASS
96	95	5	9	6.0	2121	PASS
173	174	0.00	2	1.4	411	PASS
174	95	50	120	84.7	30152	PASS
175	174	5	9	7.4	2220	PASS
176	174	95	105	95.2	28712	PASS
177	176	5	10	6.4	1842	PASS

m/z	Abundance
36.00	273.0
37.00	1555.0
38.00	1452.0
39.00	458.0
40.00	287.0
43.10	102.0
44.00	793.0
44.90	320.0
46.90	527.0
47.90	204.0
49.00	1356.0
50.00	5656.0
51.00	2048.0
52.00	170.0
54.90	132.0
56.00	457.0
57.00	1069.0
60.00	292.0
60.90	1579.0
62.00	1302.0
63.00	1283.0
64.00	181.0
65.10	138.0
67.10	126.0
68.00	3264.0
69.00	3533.0
69.90	325.0
72.00	197.0
73.00	1588.0
74.00	5914.0
75.00	16448.0
76.00	1558.0
77.00	278.0
77.90	144.0
79.00	972.0
79.90	313.0
80.90	1162.0
81.90	212.0
86.90	1803.0
88.00	1461.0
90.80	165.0
91.90	936.0
92.90	1479.0
94.00	4226.0
95.00	35168.0
96.00	2082.0
96.90	155.0
103.90	151.0
105.90	145.0
115.60	127.0
115.90	111.0
116.80	272.0
117.90	178.0
118.90	160.0
128.00	161.0
129.80	109.0
136.70	125.0
140.90	350.0
142.90	405.0
173.10	373.0
173.90	29016.0
174.90	2144.0
175.90	27424.0
176.90	1737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
40.00	220.0
44.00	374.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	307.0
37.00	1518.0
38.00	1439.0
39.00	530.0
40.00	294.0
44.00	765.0
44.90	354.0
45.70	104.0
46.90	455.0
47.90	197.0
49.00	1388.0
50.00	5930.0
51.00	2165.0
52.00	168.0
55.00	126.0
55.90	480.0
57.00	1033.0
60.00	304.0
61.00	1449.0
62.00	1358.0
63.00	1276.0
64.00	146.0
65.00	117.0
66.90	154.0
68.00	3496.0
69.00	3641.0
69.90	351.0
72.00	226.0
73.00	1662.0
74.00	6141.0
75.00	17192.0
76.00	1637.0
77.00	243.0
77.90	170.0
78.90	1067.0
79.90	335.0
80.90	1192.0
81.90	222.0
86.90	1691.0
88.00	1489.0
90.80	188.0
92.00	983.0
92.90	1570.0
94.00	4347.0
95.00	36640.0
96.00	2166.0
96.90	118.0
103.90	163.0
105.70	172.0
116.00	135.0
116.80	266.0
117.90	169.0
119.00	160.0
127.80	179.0
129.70	118.0
136.70	116.0
140.90	363.0
142.90	467.0
147.70	115.0
154.80	126.0
172.00	117.0
173.00	431.0
173.90	31256.0
174.90	2320.0
175.90	29696.0
176.90	1862.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	286.0
37.00	1357.0
38.00	1295.0
38.90	562.0
40.00	265.0
43.90	742.0
45.00	317.0
46.90	335.0
47.80	200.0
49.00	1277.0
50.00	5750.0
51.00	2012.0
52.00	150.0
55.00	146.0
55.90	463.0
57.00	914.0
60.00	256.0
61.00	1324.0
62.00	1314.0
63.00	1129.0
63.90	105.0
64.90	116.0
66.80	184.0
68.00	3350.0
69.00	3427.0
69.90	346.0
72.00	211.0
73.00	1600.0
74.00	5705.0
75.00	16480.0
76.00	1569.0
77.00	189.0
77.90	191.0
78.90	1038.0
79.90	376.0
80.90	1110.0
81.90	217.0
86.90	1470.0
88.00	1320.0
90.80	180.0
92.00	916.0
92.90	1458.0
94.00	4091.0
95.00	35040.0
96.00	2115.0
103.90	158.0
105.70	204.0
115.80	131.0
116.70	258.0
118.00	128.0
119.00	155.0
127.80	177.0
129.70	131.0
140.80	312.0
142.80	457.0
154.80	145.0
171.90	136.0
173.00	429.0
173.90	30184.0
174.90	2197.0
175.90	29016.0
176.90	1927.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206