




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026799.D
 Acq On : 15 Jul 2022 18:37
 Operator : SY/MD
 Sample : N3710-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B09

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:57:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

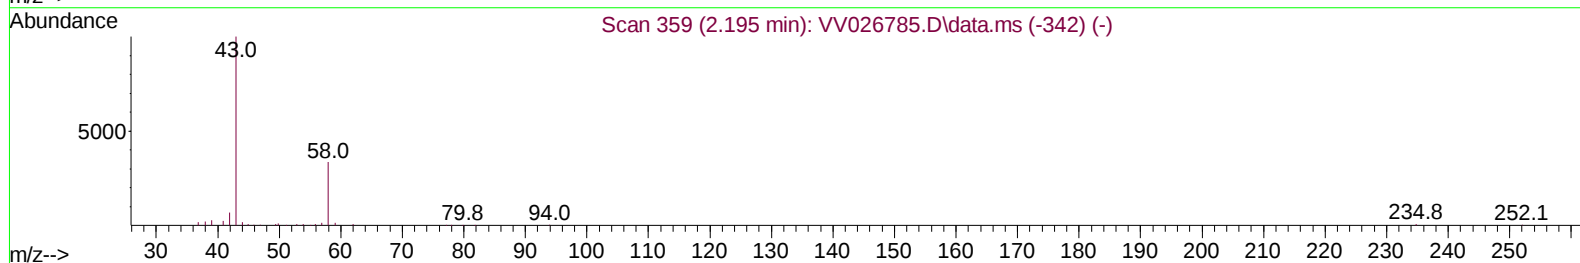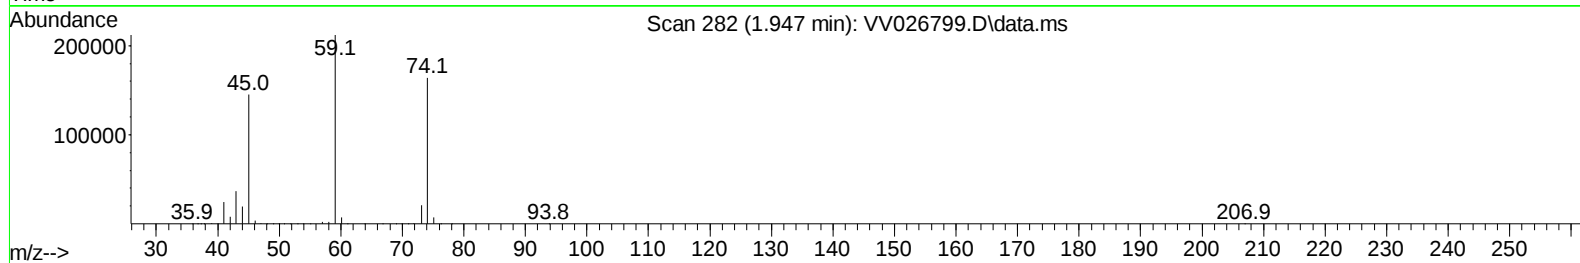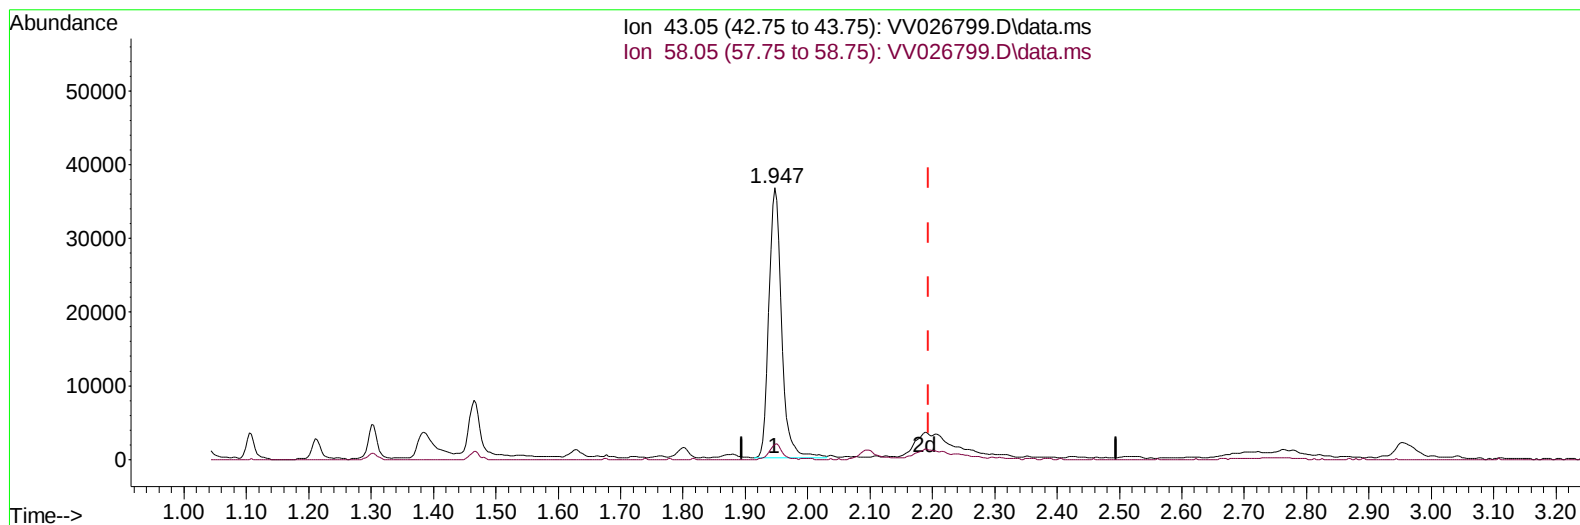

TIC: VV026799.D\data.ms

(13) Acetone (T)

1.947min (-0.248) 17.72 ug/L

response 52548

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	10.30	5.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026799.D
Acq On : 15 Jul 2022 18:37
Operator : SY/MD
Sample : N3710-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B09

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:57:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

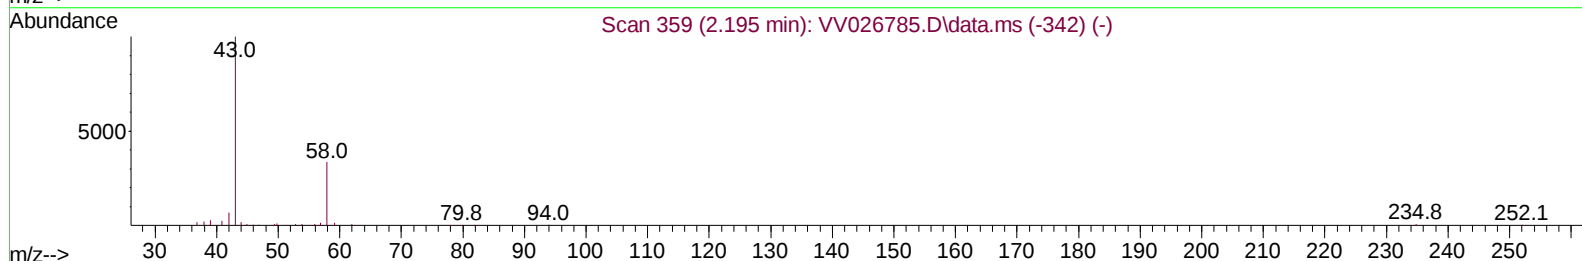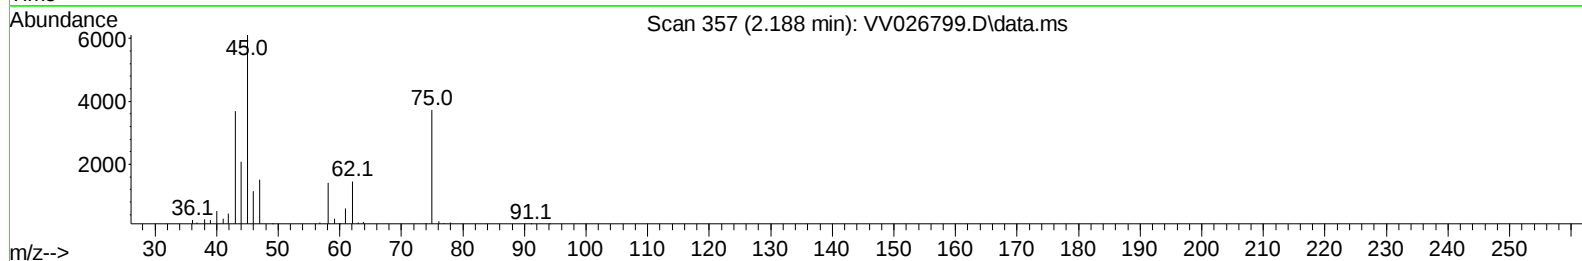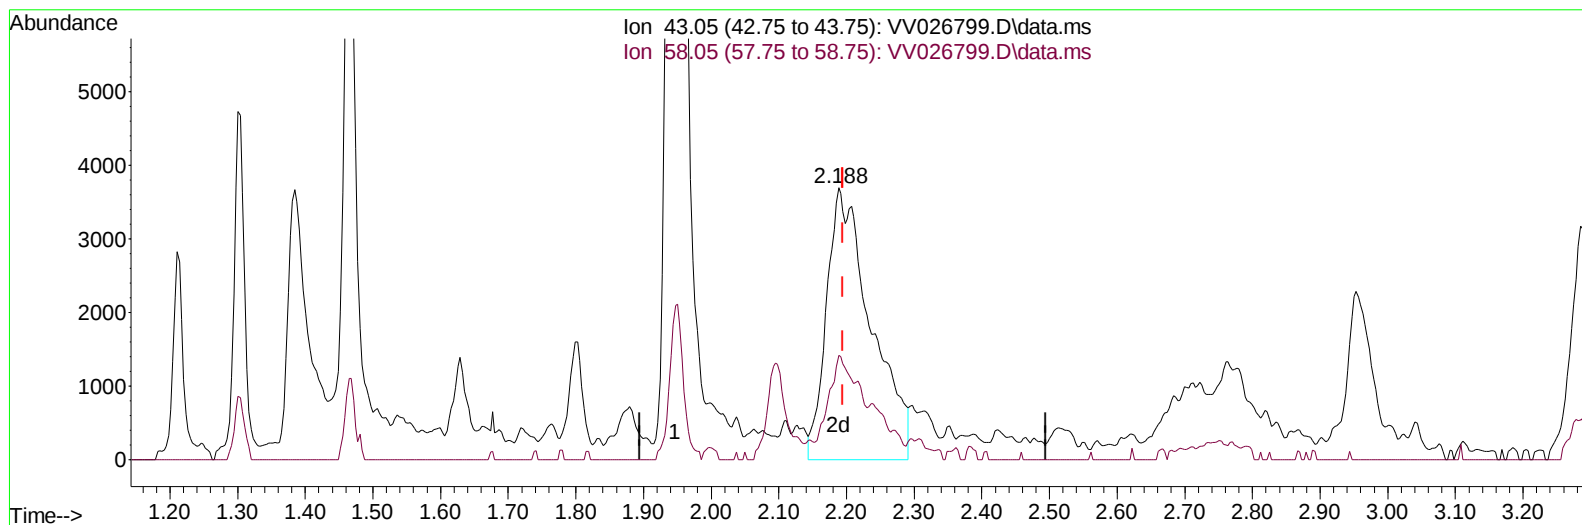

TIC: VV026799.D\data.ms

(13) Acetone (T)

2.188min (-0.006) 5.69 ug/L m

response 16864

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	10.30	17.81
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026799.D
 Acq On : 15 Jul 2022 18:37
 Operator : SY/MD
 Sample : N3710-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B09

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:57:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	247534	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	231243	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	119139	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	53902	2.387	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	47.800%	
7) Chloroethane-d5	1.561	69	60230	3.087	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	61.800%#	
11) 1,1-Dichloroethene-d2	2.101	63	79309	1.829	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	36.600%#	
20) 2-Butanone-d5	3.902	46	211626	60.045	ug/L	-0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	120.080%	
24) Chloroform-d	4.342	84	132020	3.343	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	66.800%#	
26) 1,2-Dichloroethane-d4	5.031	65	75252	4.362	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	87.200%	
32) Benzene-d6	5.047	84	255072	3.630	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	72.600%	
36) 1,2-Dichloropropane-d6	6.069	67	92565	4.394	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	87.800%	
41) Toluene-d8	7.313	98	171203	2.745	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	54.800%#	
43) trans-1,3-Dichloroprop...	7.625	79	23641	3.430	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	68.600%	
46) 2-Hexanone-d5	8.088	63	164330	55.064	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	110.120%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	81765	4.982	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	89646	4.319	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	86.400%	
Target Compounds						
					Qvalue	
13) Acetone	2.188	43	16864m	5.687	ug/L	
14) Carbon disulfide	2.288	76	18015	0.282	ug/L	99
17) Methyl tert-butyl Ether	2.767	73	7138	0.191	ug/L #	84
25) Chloroform	4.371	83	22414	0.587	ug/L	99
33) Benzene	5.098	78	158452	2.050	ug/L	100
42) Toluene	7.394	91	20842	0.267	ug/L	95
51) Chlorobenzene	8.879	112	322202	6.527	ug/L	99
52) Ethylbenzene	9.018	91	11187	0.145	ug/L	96
53) m,p-Xylene	9.140	106	4810	0.160	ug/L	86
54) o-Xylene	9.548	106	4348	0.152	ug/L	100
55) Styrene	9.567	104	2776	0.055	ug/L	89
60) Isopropylbenzene	9.931	105	34427	0.463	ug/L	99
62) 1,3,5-Trimethylbenzene	10.538	105	6474	0.110	ug/L	98
63) 1,2,4-Trimethylbenzene	10.915	105	22716	0.378	ug/L	99
65) 1,4-Dichlorobenzene	11.271	146	33467	0.904	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_V

ClientSampleId :

H0B09

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/18/2022

Supervised By :Mahesh Dadoda 07/18/2022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026799.D
Acq On : 15 Jul 2022 18:37
Operator : SY/MD
Sample : N3710-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B09

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:57:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

