

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026786.D
 Acq On : 15 Jul 2022 13:16
 Operator : SY/MD
 Sample : VV0715WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK395

Quant Time: Jul 16 00:54:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	212545	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	217454	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	85664	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	91783	4.733	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.600%
7) Chloroethane-d5	1.558	69	81936	4.891	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.800%
11) 1,1-Dichloroethene-d2	2.098	63	125315	3.366	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.400%
20) 2-Butanone-d5	3.912	46	146255	48.328	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.660%
24) Chloroform-d	4.342	84	172722	5.094	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
26) 1,2-Dichloroethane-d4	5.031	65	77547	5.235	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%
32) Benzene-d6	5.043	84	301300	4.560	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
36) 1,2-Dichloropropane-d6	6.066	67	100623	5.079	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.600%
41) Toluene-d8	7.313	98	216207	3.686	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.800%
43) trans-1,3-Dichloroprop...	7.622	79	27593	4.257	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.091	63	105196	37.485	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.960%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	71227	4.615	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	76788	5.145	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds						
16) Methylene chloride	2.497	84	10729	0.483	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026786.D
Acq On : 15 Jul 2022 13:16
Operator : SY/MD
Sample : VV0715WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Time: Jul 16 00:54:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

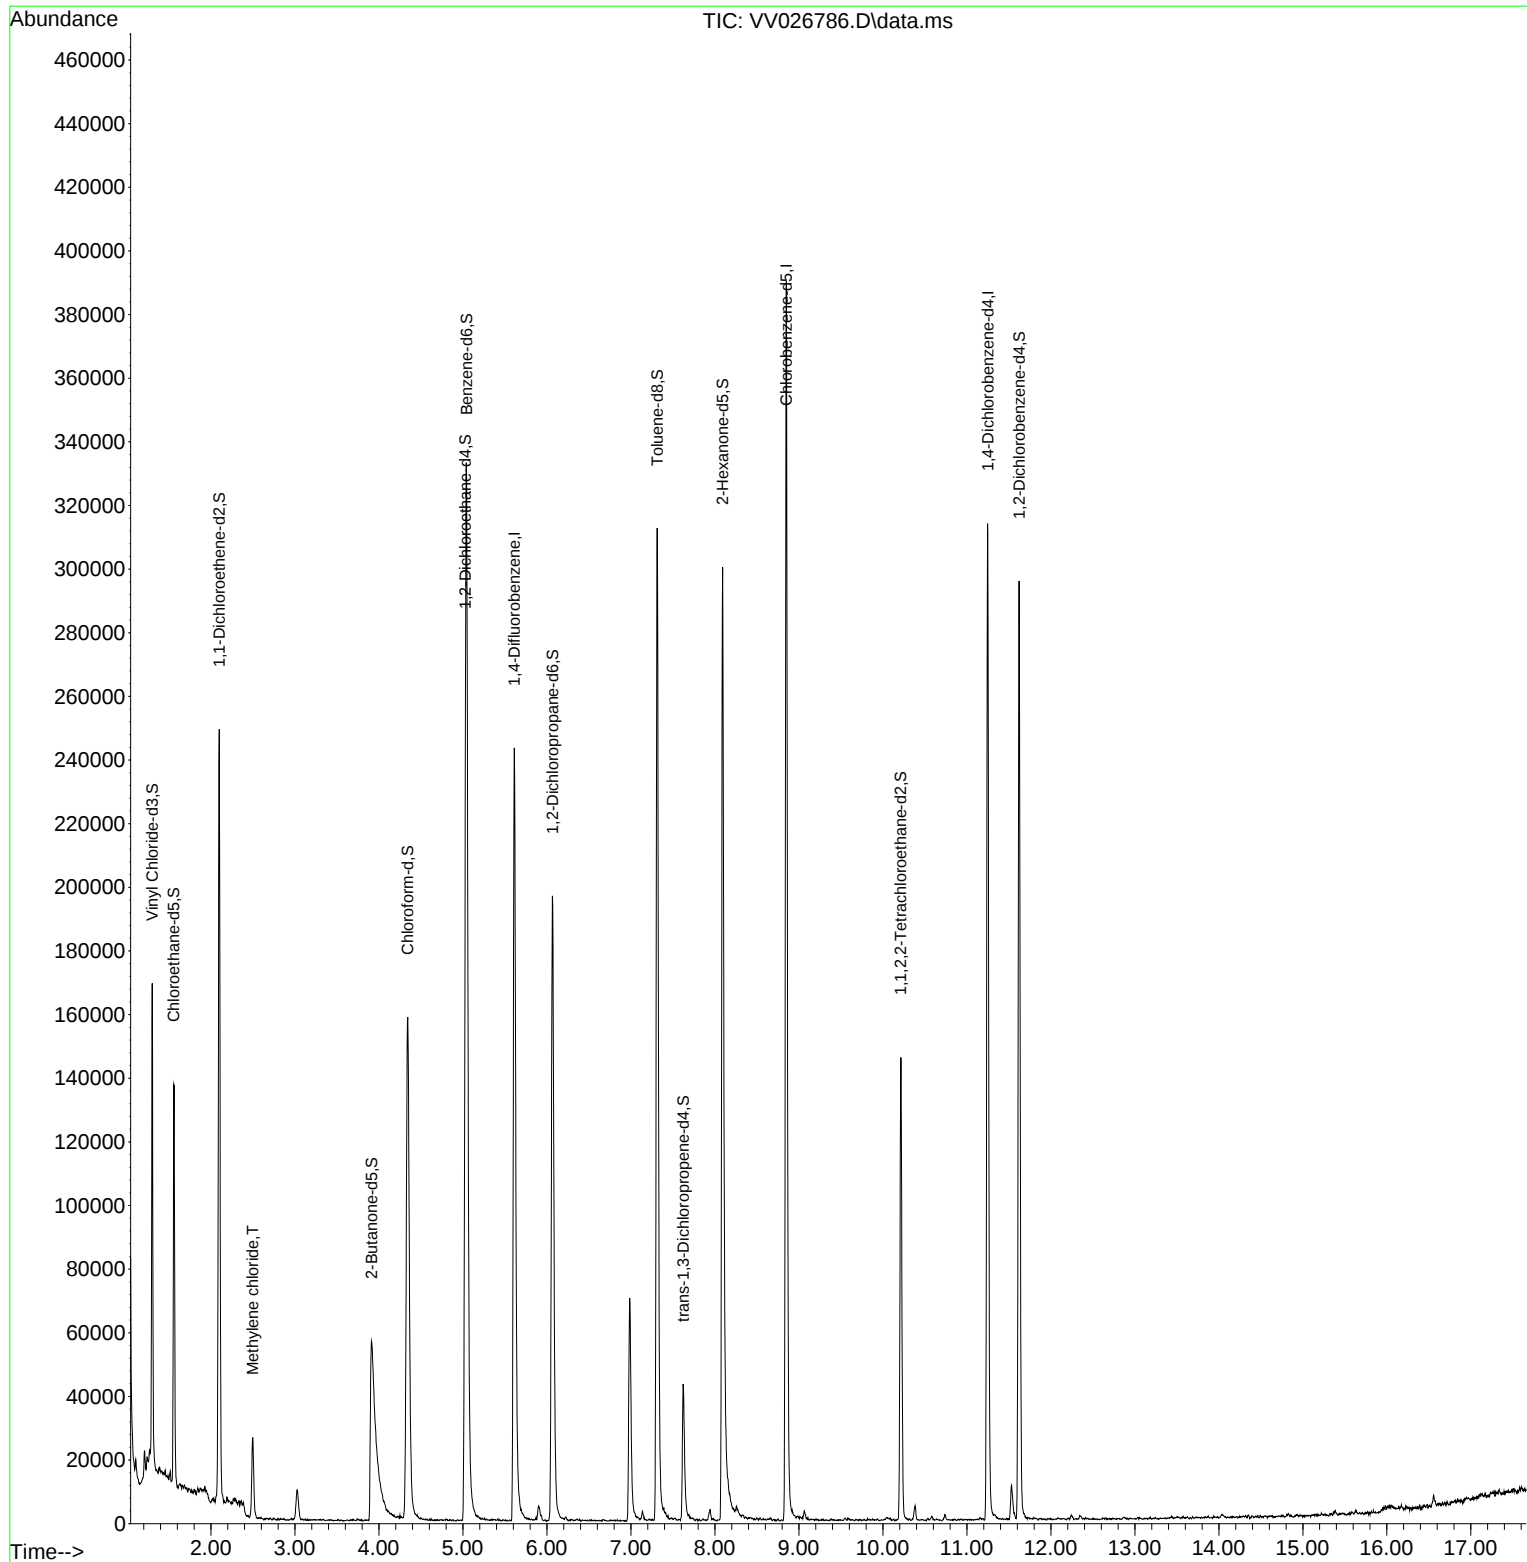

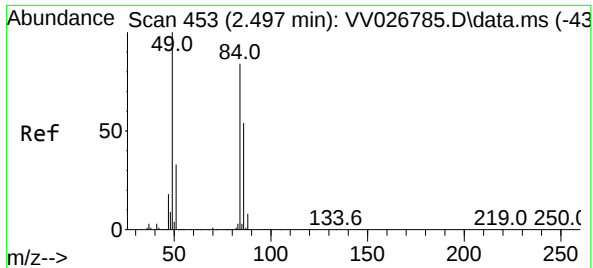

#16
Methylene chloride
Concen: 0.483 ug/L
RT: 2.497 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV026786.D
Acq: 15 Jul 2022 13:16

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Tgt Ion:	84	Resp:	10729
Ion	Ratio	Lower	Upper
84	100		
86	63.3	44.8	83.2
49	106.2	78.7	146.1

