

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071522\
 Data File : VW026791.D
 Acq On : 15 Jul 2022 15:19
 Operator : SY/MD
 Sample : N3710-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B51

Quant Time: Jul 16 00:55:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	223175	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	231194	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	90210	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	59644	2.929	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	58.600%
7) Chloroethane-d5	1.561	69	61563	3.499	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.000%
11) 1,1-Dichloroethene-d2	2.101	63	83356	2.133	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	42.600%#
20) 2-Butanone-d5	3.889	46	143004	45.003	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.000%
24) Chloroform-d	4.346	84	149746	4.206	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
26) 1,2-Dichloroethane-d4	5.031	65	68739	4.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.400%
32) Benzene-d6	5.047	84	240684	3.426	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	68.600%#
36) 1,2-Dichloropropane-d6	6.066	67	88102	4.183	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.600%
41) Toluene-d8	7.313	98	170731	2.738	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	54.800%#
43) trans-1,3-Dichloroprop...	7.625	79	23591	3.423	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.400%
46) 2-Hexanone-d5	8.088	63	130224	43.645	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.300%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	73006	4.449	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	68090	4.332	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds						Qvalue
13) Acetone	2.179	43	12353	4.620	ug/L #	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026791.D
Acq On : 15 Jul 2022 15:19
Operator : SY/MD
Sample : N3710-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B51

Quant Time: Jul 16 00:55:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

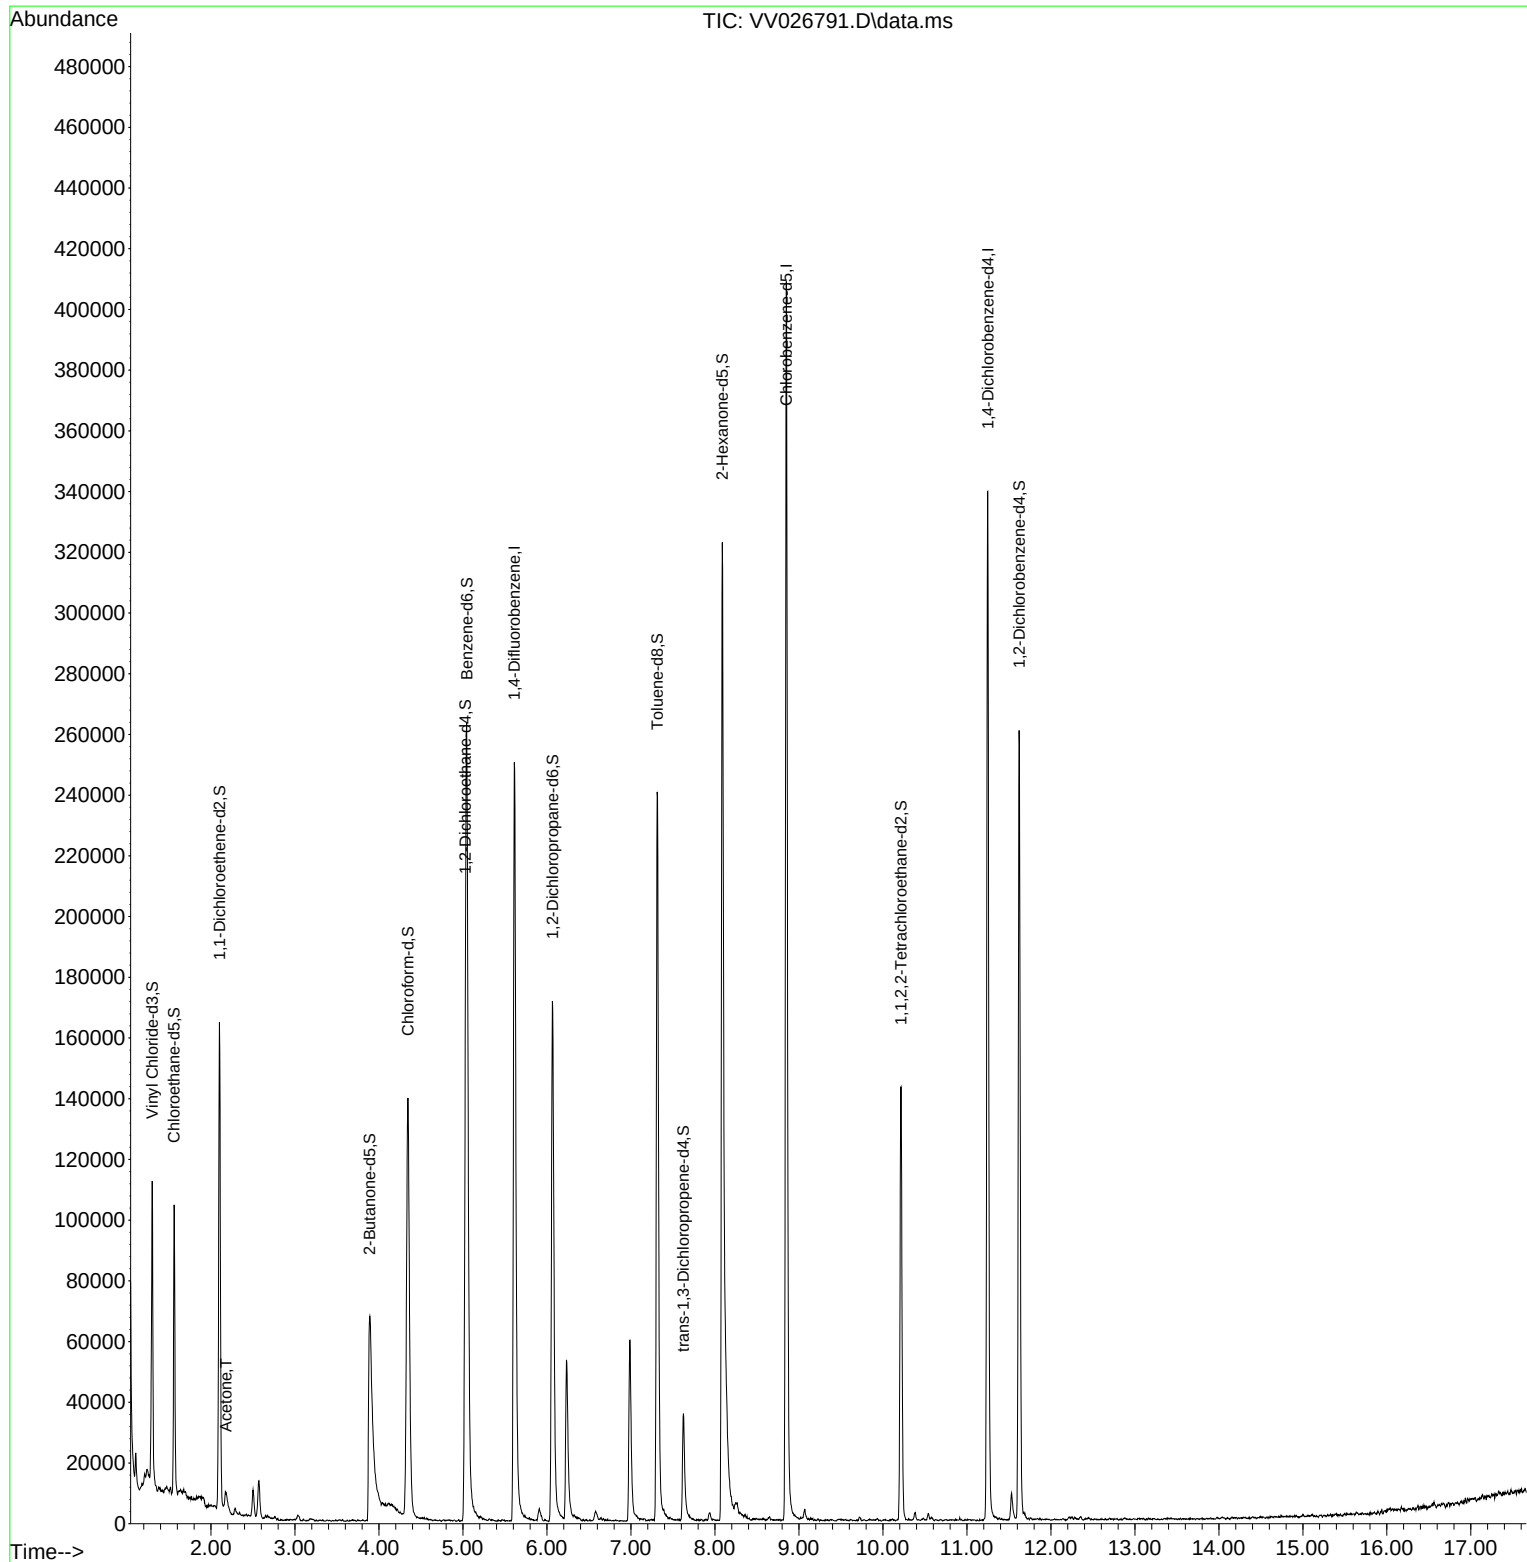

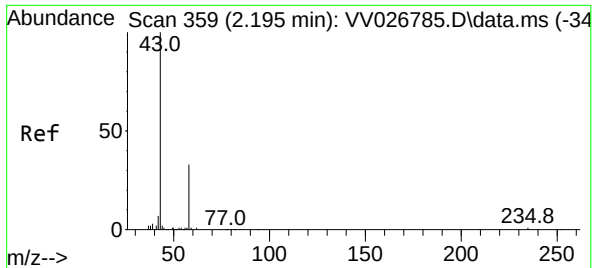

#13
 Acetone
 Concen: 4.620 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV026791.D
 Acq: 15 Jul 2022 15:19

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B51

Tgt Ion: 43 Resp: 12353
 Ion Ratio Lower Upper
 43 100
 58 37.1 0.0 20.6#

