

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071522\
 Data File : VW026792.D
 Acq On : 15 Jul 2022 15:43
 Operator : SY/MD
 Sample : N3710-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B46

Quant Time: Jul 16 00:55:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	219772	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	228889	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	89758	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	58527	2.919	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	58.400%	
7) Chloroethane-d5	1.564	69	62102	3.585	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.600%	
11) 1,1-Dichloroethene-d2	2.101	63	82738	2.150	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	43.000%#	
20) 2-Butanone-d5	3.892	46	152834	48.841	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.680%	
24) Chloroform-d	4.342	84	153463	4.377	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	5.030	65	70065	4.575	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
32) Benzene-d6	5.046	84	244373	3.514	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	70.200%	
36) 1,2-Dichloropropane-d6	6.069	67	89863	4.309	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.200%	
41) Toluene-d8	7.316	98	168157	2.724	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	54.400%#	
43) trans-1,3-Dichloroprop...	7.625	79	24572	3.602	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	72.000%	
46) 2-Hexanone-d5	8.088	63	133819	45.302	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.600%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	76864	4.731	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	70789	4.526	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	90.600%	
Target Compounds						Qvalue
13) Acetone	2.178	43	16401	6.229	ug/L	# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026792.D
Acq On : 15 Jul 2022 15:43
Operator : SY/MD
Sample : N3710-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B46

Quant Time: Jul 16 00:55:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

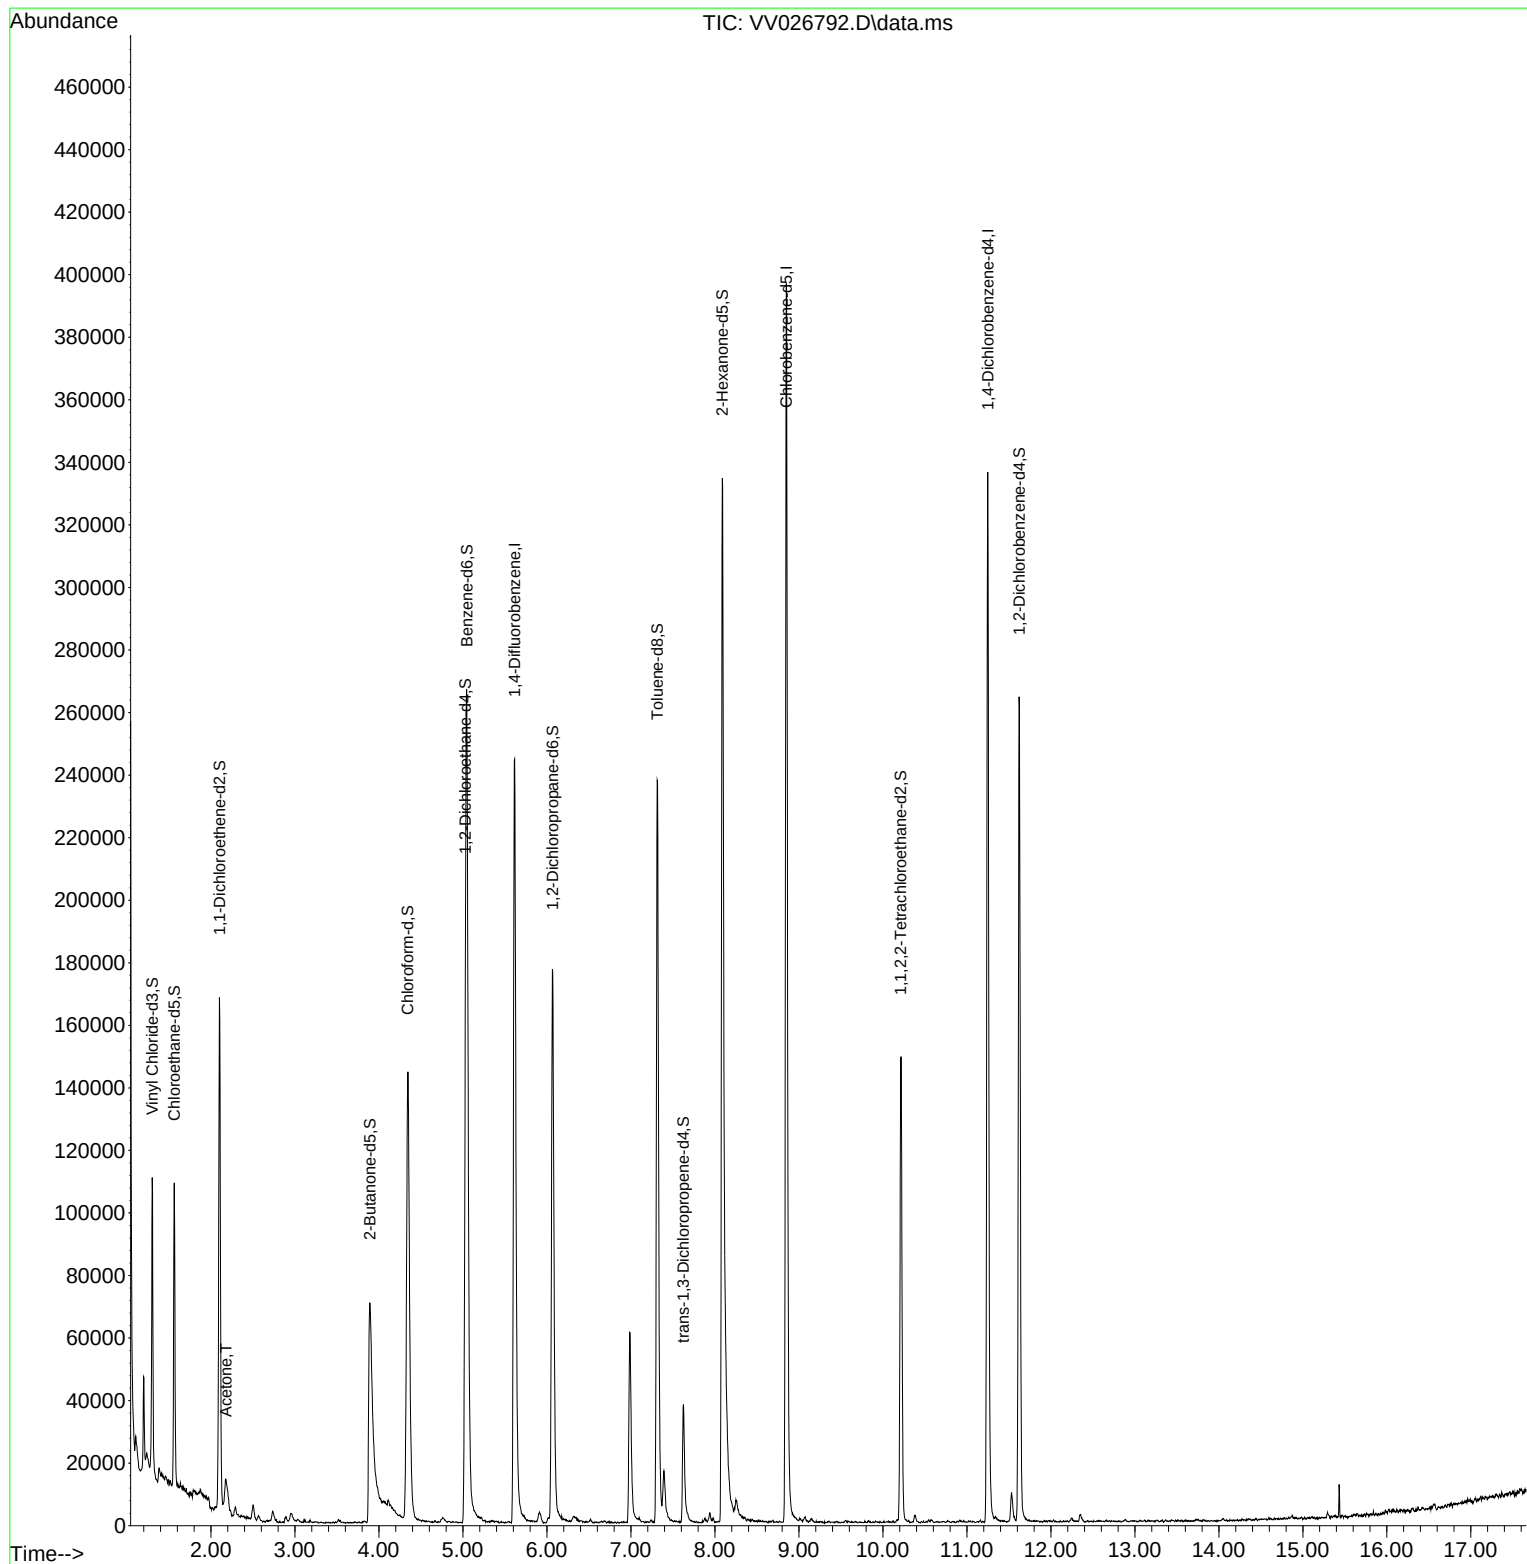

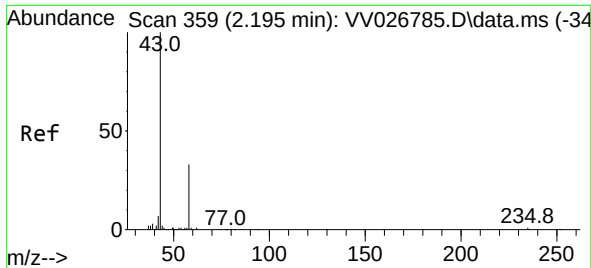

#13
 Acetone
 Concen: 6.229 ug/L
 RT: 2.178 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV026792.D
 Acq: 15 Jul 2022 15:43

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B46

Tgt Ion: 43 Resp: 16401
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 20.6#

