

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071522\
 Data File : VW026793.D
 Acq On : 15 Jul 2022 16:08
 Operator : SY/MD
 Sample : N3710-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B47

Quant Time: Jul 16 00:55:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	218065	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	226909	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	87629	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	58804	2.956	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	59.200%	
7) Chloroethane-d5	1.561	69	65790	3.827	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	76.600%	
11) 1,1-Dichloroethene-d2	2.101	63	86970	2.277	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	45.600%#	
20) 2-Butanone-d5	3.902	46	178634	57.533	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.060%	
24) Chloroform-d	4.342	84	159275	4.579	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	5.030	65	72954	4.801	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.000%	
32) Benzene-d6	5.047	84	254577	3.692	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	73.800%	
36) 1,2-Dichloropropane-d6	6.069	67	93388	4.517	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.400%	
41) Toluene-d8	7.317	98	172013	2.810	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	56.200%#	
43) trans-1,3-Dichloroprop...	7.625	79	25643	3.791	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	75.800%	
46) 2-Hexanone-d5	8.088	63	140777	48.073	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.140%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	77187	4.793	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	73275	4.799	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.000%	
Target Compounds						
13) Acetone	2.185	43	14014	5.364	ug/L	Qvalue # 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026793.D
Acq On : 15 Jul 2022 16:08
Operator : SY/MD
Sample : N3710-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B47

Quant Time: Jul 16 00:55:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

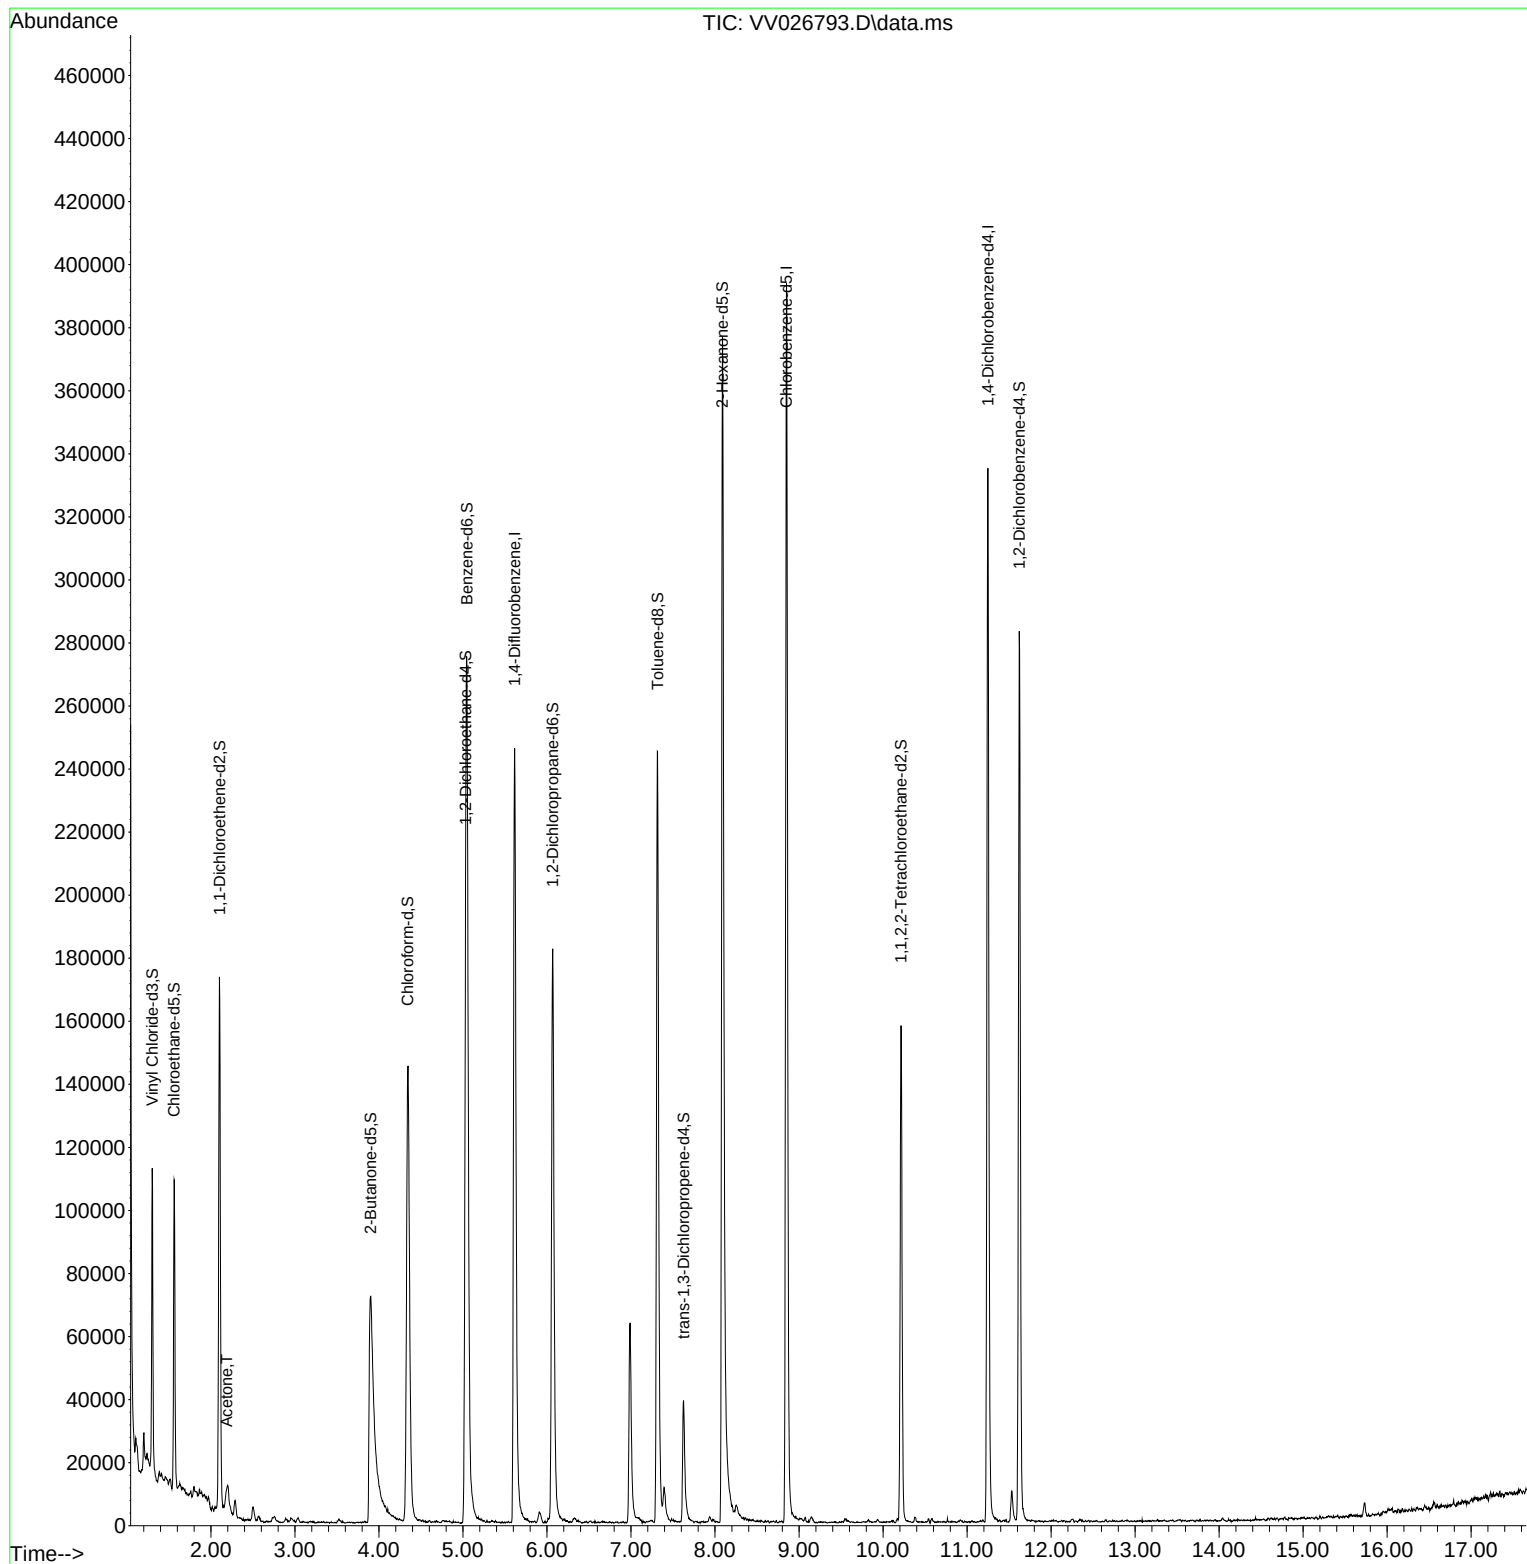

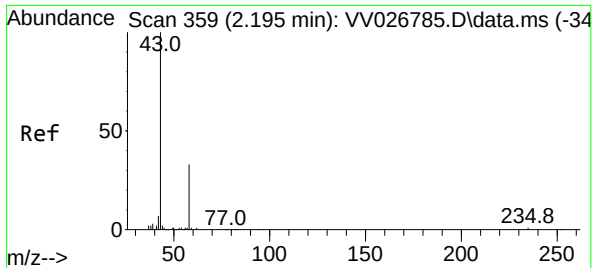

#13
 Acetone
 Concen: 5.364 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV026793.D
 Acq: 15 Jul 2022 16:08

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B47

Tgt Ion: 43 Resp: 14014
 Ion Ratio Lower Upper
 43 100
 58 30.7 0.0 20.6#

