

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071522\
 Data File : VW026794.D
 Acq On : 15 Jul 2022 16:33
 Operator : SY/MD
 Sample : N3710-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B53

Quant Time: Jul 16 00:56:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	225938	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	237563	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	93104	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	59803	2.901	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	58.000%
7) Chloroethane-d5	1.561	69	65694	3.689	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.800%
11) 1,1-Dichloroethene-d2	2.101	63	87677	2.216	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	44.400%#
20) 2-Butanone-d5	3.899	46	192256	59.763	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.520%
24) Chloroform-d	4.346	84	155847	4.324	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	5.027	65	74311	4.720	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.047	84	252333	3.496	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	70.000%
36) 1,2-Dichloropropane-d6	6.066	67	94052	4.345	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.000%
41) Toluene-d8	7.313	98	174011	2.716	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	54.400%#
43) trans-1,3-Dichloroprop...	7.625	79	25116	3.547	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.000%
46) 2-Hexanone-d5	8.088	63	137908	44.981	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.960%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	77094	4.572	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	71715	4.421	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.400%
Target Compounds						
					Qvalue	
13) Acetone	2.185	43	11689	4.319	ug/L #	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026794.D
Acq On : 15 Jul 2022 16:33
Operator : SY/MD
Sample : N3710-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B53

Quant Time: Jul 16 00:56:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

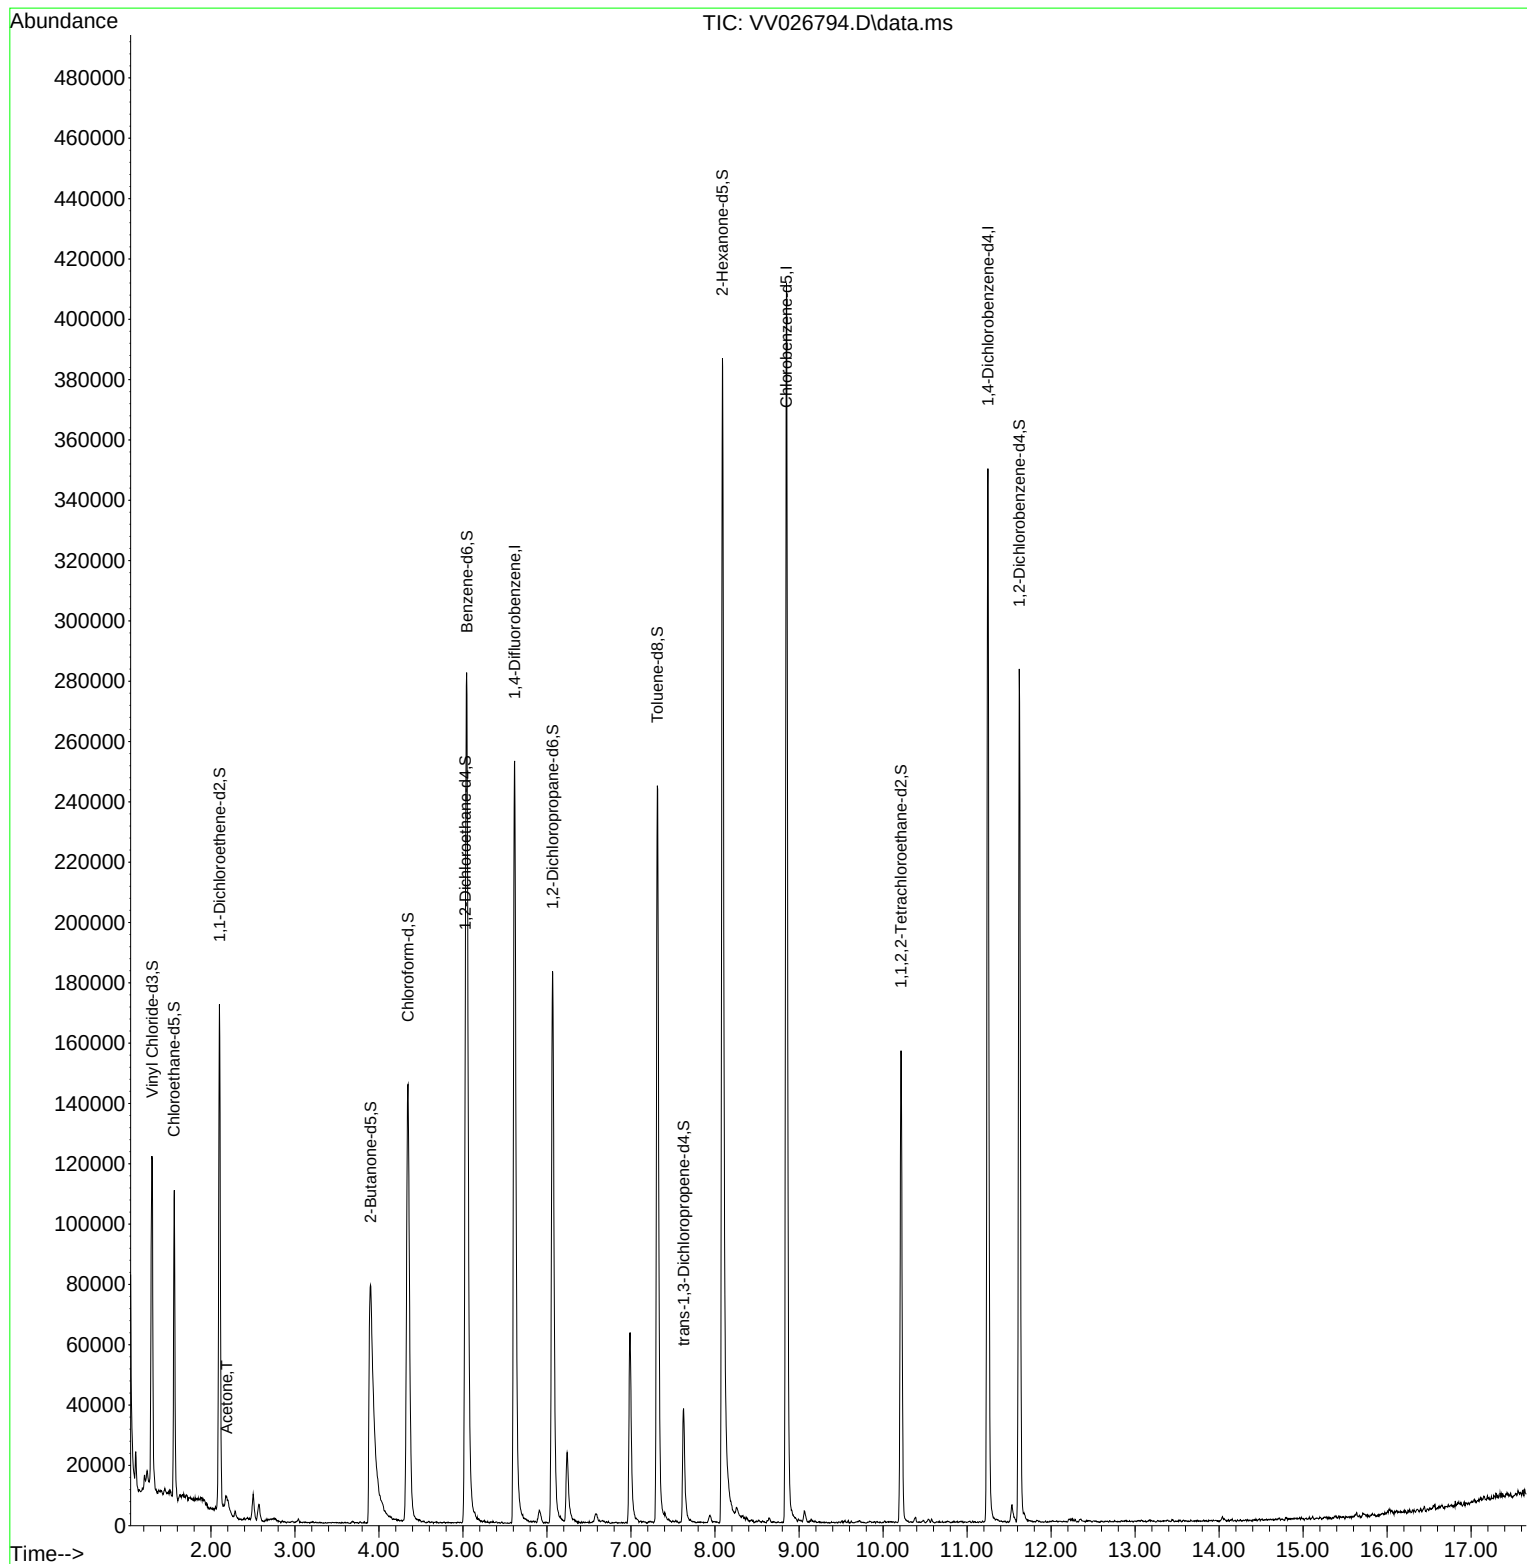

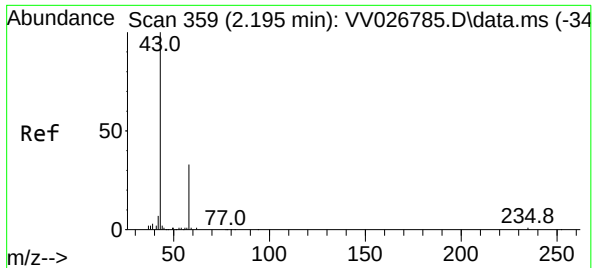

#13
 Acetone
 Concen: 4.319 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV026794.D
 Acq: 15 Jul 2022 16:33

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B53

Tgt Ion: 43 Resp: 11689
 Ion Ratio Lower Upper
 43 100
 58 38.2 0.0 20.6#

