

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071522\
 Data File : VW026797.D
 Acq On : 15 Jul 2022 17:47
 Operator : SY/MD
 Sample : N3710-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B41

Quant Time: Jul 16 00:56:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 16 00:49:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	222804	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	233134	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	91723	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	58202	2.863	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	57.200%	
7) Chloroethane-d5	1.561	69	64149	3.653	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	73.000%	
11) 1,1-Dichloroethene-d2	2.101	63	83682	2.144	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	42.800%#	
20) 2-Butanone-d5	3.902	46	193958	61.140	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	122.280%	
24) Chloroform-d	4.346	84	154631	4.351	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.000%	
26) 1,2-Dichloroethane-d4	5.031	65	71282	4.591	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.800%	
32) Benzene-d6	5.047	84	246345	3.477	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	69.600%#	
36) 1,2-Dichloropropane-d6	6.069	67	94072	4.429	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.600%	
41) Toluene-d8	7.313	98	168991	2.687	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	53.800%#	
43) trans-1,3-Dichloroprop...	7.625	79	24778	3.566	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	71.400%	
46) 2-Hexanone-d5	8.088	63	142513	47.366	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.740%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	78411	4.739	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	71479	4.473	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	89.400%	
Target Compounds					Qvalue	
13) Acetone	2.185	43	28885	10.822	ug/L #	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026797.D
Acq On : 15 Jul 2022 17:47
Operator : SY/MD
Sample : N3710-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B41

Quant Time: Jul 16 00:56:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 16 00:49:45 2022
Response via : Initial Calibration

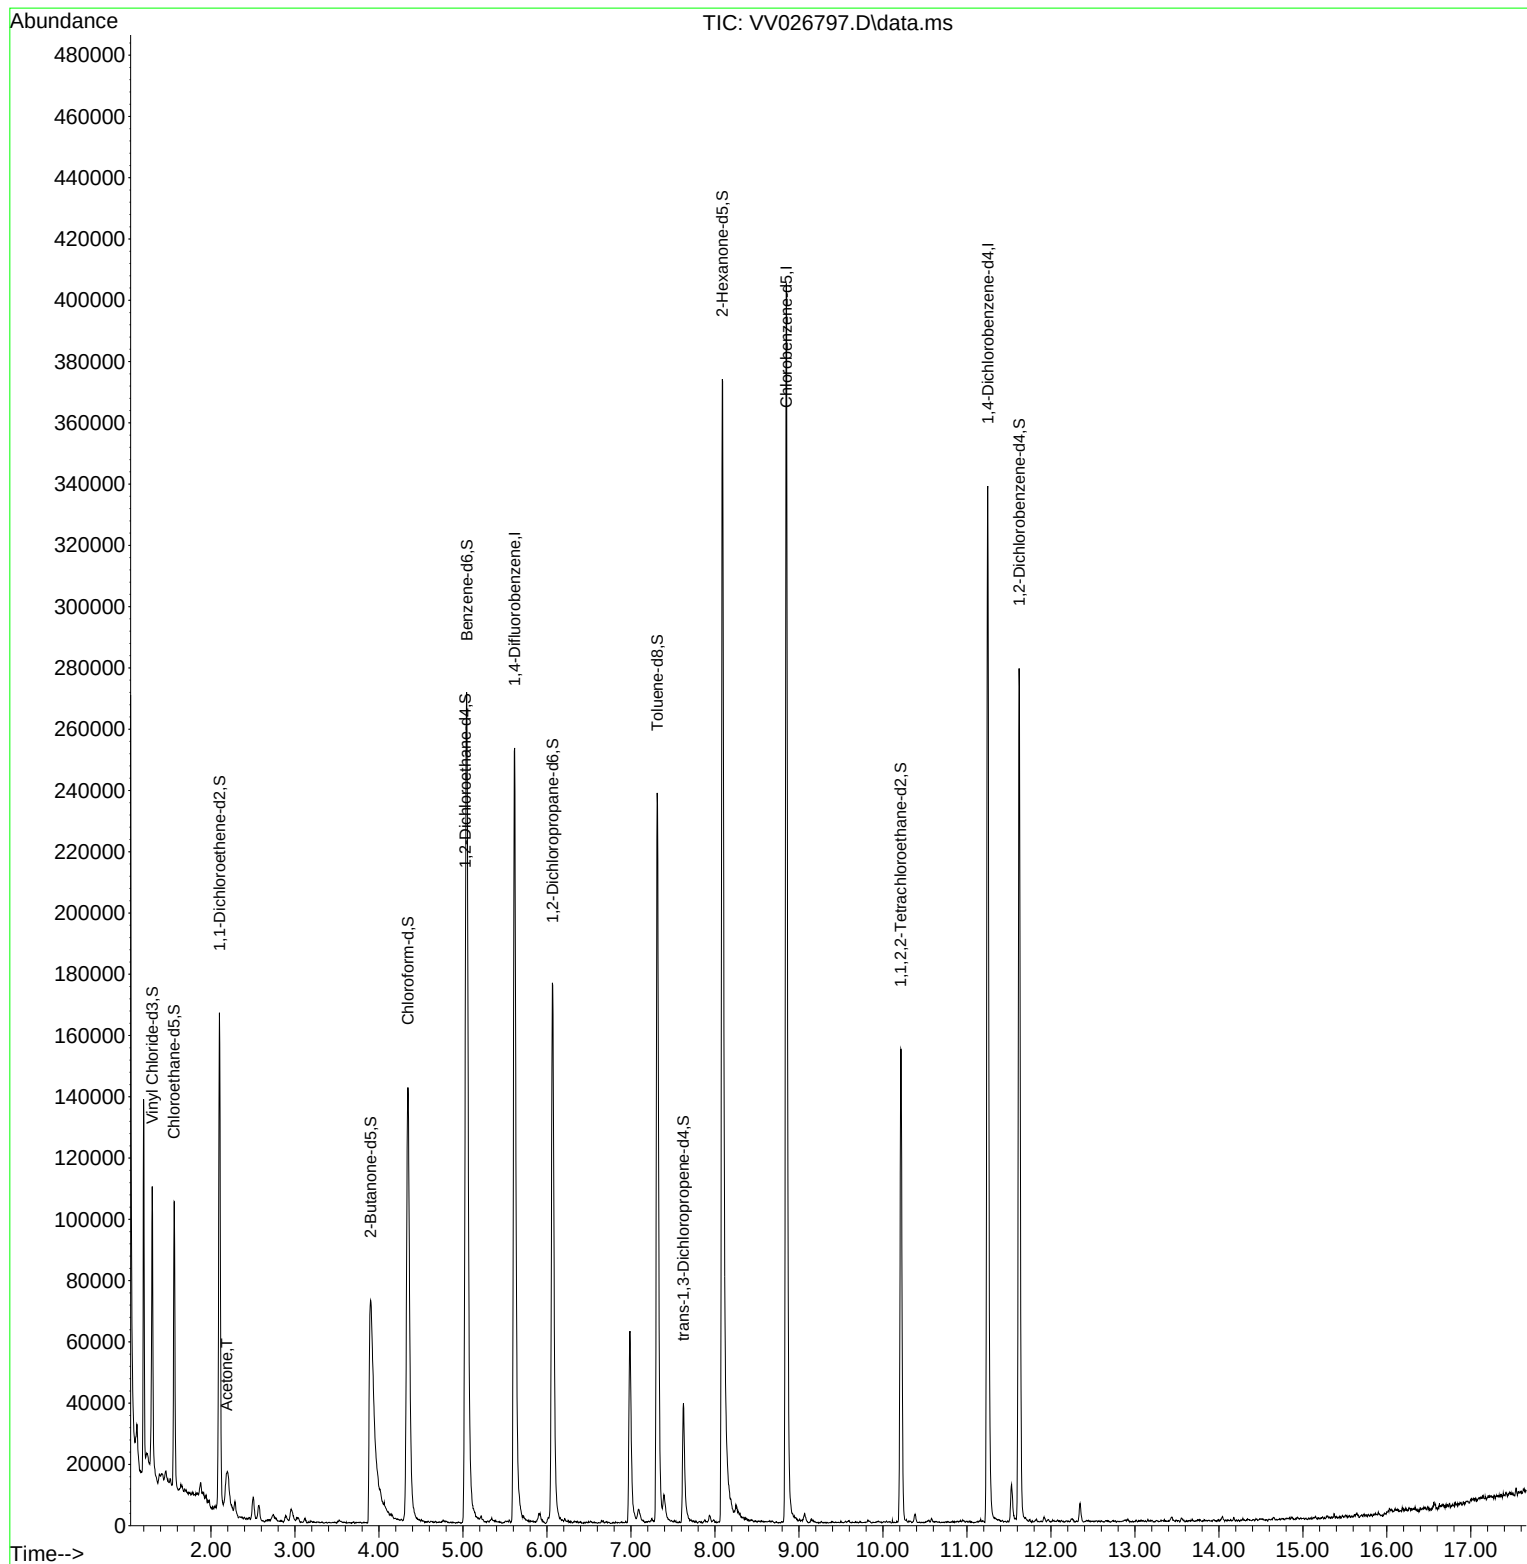

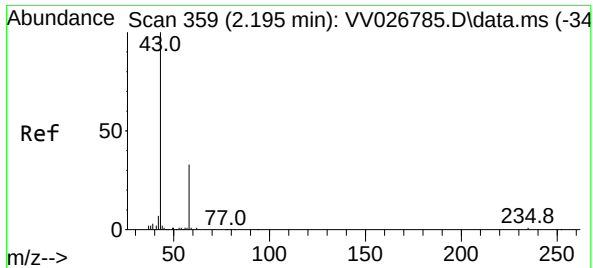

#13
 Acetone
 Concen: 10.822 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV026797.D
 Acq: 15 Jul 2022 17:47

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B41

Tgt Ion: 43 Resp: 28885
 Ion Ratio Lower Upper
 43 100
 58 32.9 0.0 20.6#

