

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026786.D
 Acq On : 15 Jul 2022 13:16
 Operator : SY/MD
 Sample : VV0715WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK395

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	48	53	58	rBV2	8177	9117	1.12%	0.145%
2	1.301	75	81	103	rVB	153968	156547	19.25%	2.489%
3	1.558	154	161	175	rVB	126802	146145	17.97%	2.324%
4	2.098	319	329	341	rBV	240892	333855	41.05%	5.308%
5	2.497	440	453	468	rVB	25288	41915	5.15%	0.666%
6	3.027	604	618	632	rVB4	9427	20150	2.48%	0.320%
7	3.912	883	893	938	rBV2	56484	259398	31.90%	4.124%
8	4.342	1010	1027	1061	rBV2	157338	403440	49.61%	6.415%
9	5.040	1228	1244	1280	rBV2	332467	813249	100.00%	12.931%
10	5.613	1410	1422	1446	rBV	242937	500566	61.55%	7.959%
11	6.066	1549	1563	1593	rBV	196288	414526	50.97%	6.591%
12	6.985	1837	1849	1874	rBV	70215	138398	17.02%	2.201%
13	7.313	1939	1951	1973	rBV	311839	556154	68.39%	8.843%
14	7.622	2037	2047	2065	rBV2	42831	79865	9.82%	1.270%
15	8.091	2180	2193	2218	rBV	299449	572512	70.40%	9.103%
16	8.850	2415	2429	2449	rBV	389482	634964	78.08%	10.096%
17	10.214	2840	2853	2870	rBV	145336	226434	27.84%	3.600%
18	11.246	3162	3174	3195	rBV	313211	498653	61.32%	7.929%
19	11.532	3254	3263	3272	rBV3	10858	19172	2.36%	0.305%
20	11.622	3280	3291	3308	rBV	294722	464171	57.08%	7.380%




Sum of corrected areas: 6289231

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026786.D
Acq On : 15 Jul 2022 13:16
Operator : SY/MD
Sample : VV0715WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

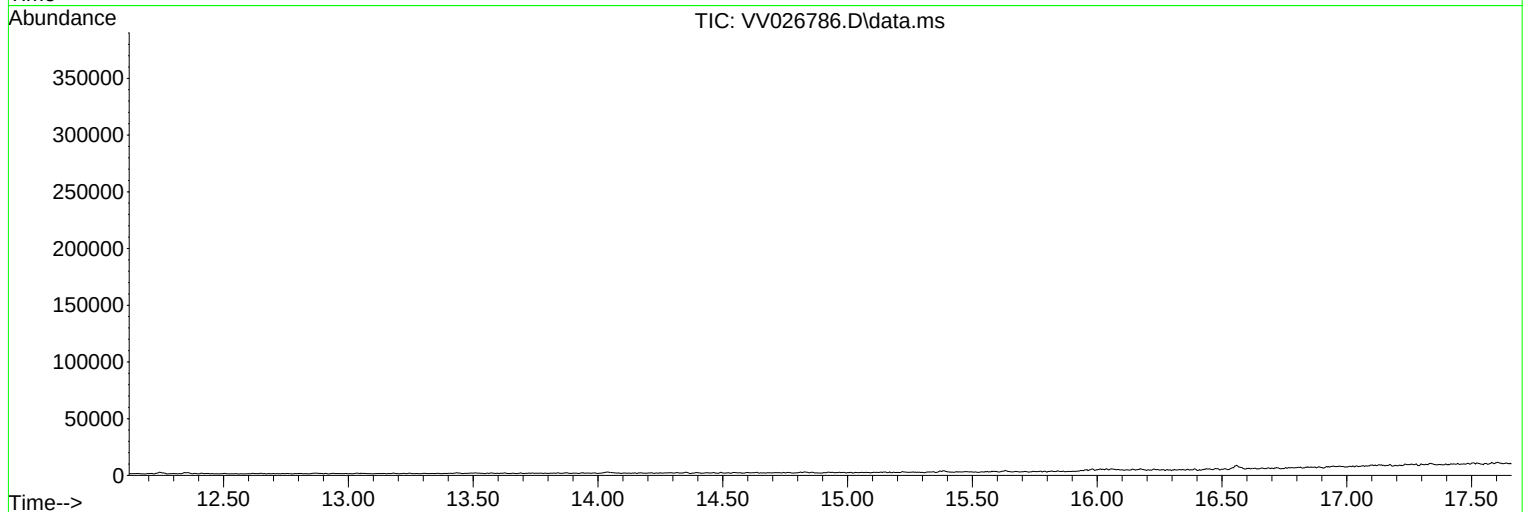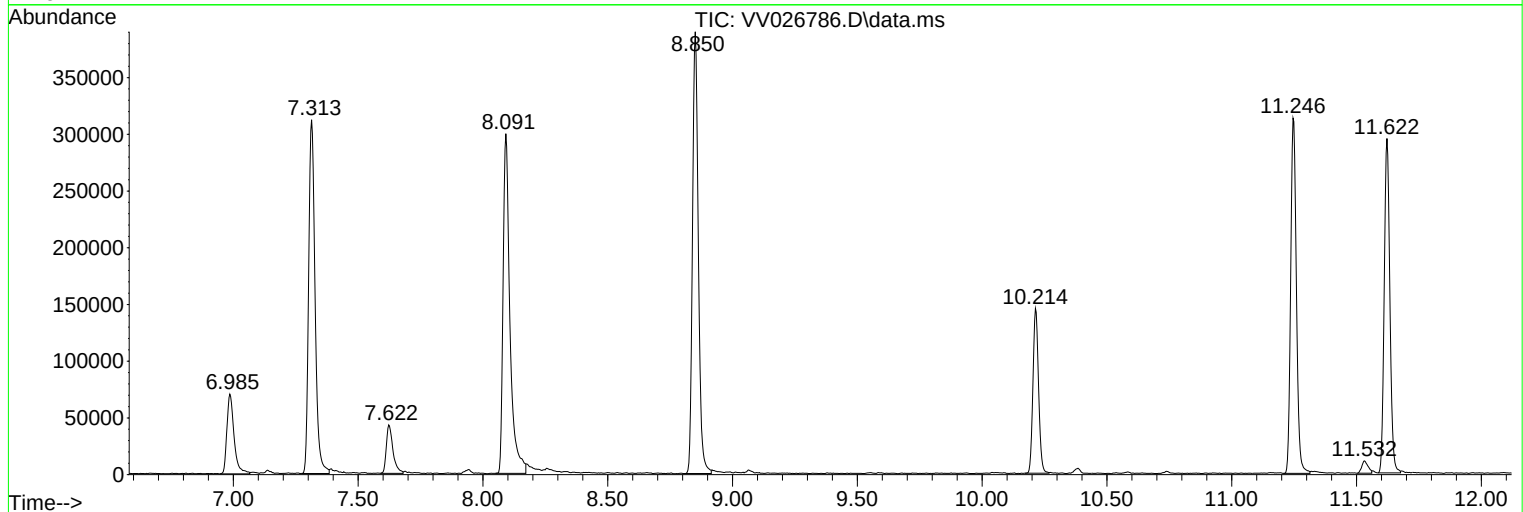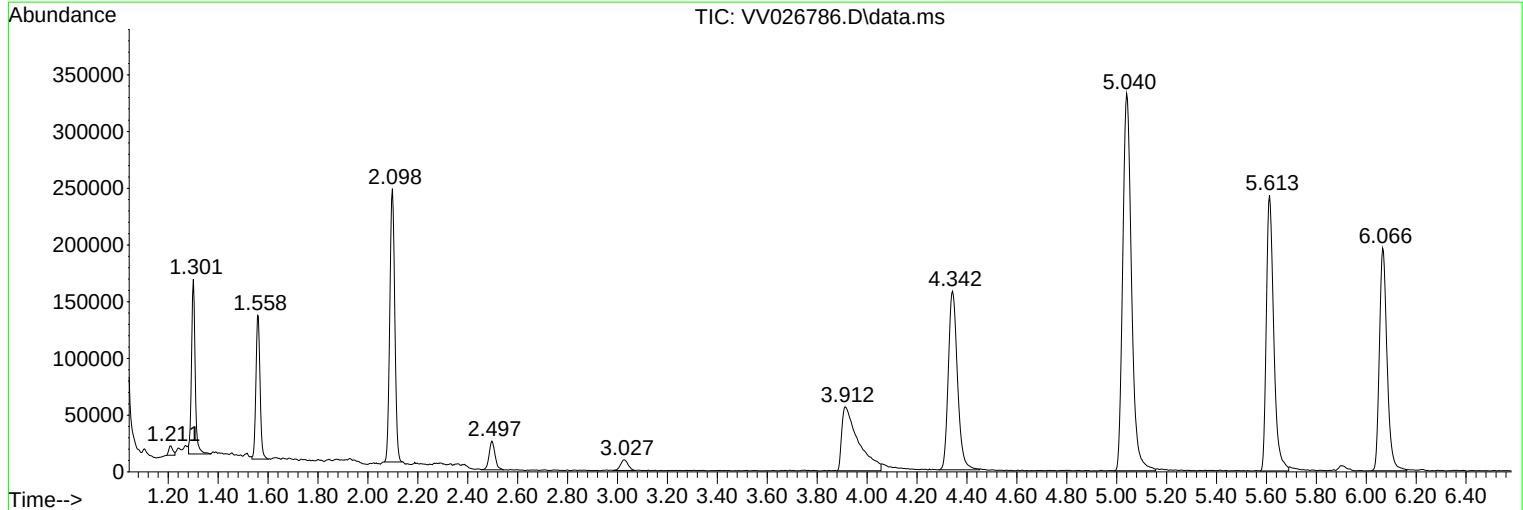

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026786.D
Acq On : 15 Jul 2022 13:16
Operator : SY/MD
Sample : VV0715WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026786.D
Acq On : 15 Jul 2022 13:16
Operator : SY/MD
Sample : VV0715WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc