

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026787.D
 Acq On : 15 Jul 2022 13:39
 Operator : SY/MD
 Sample : N3670-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT2-2022-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	22	25	31	rVB	10126	8481	1.14%	0.129%
2	1.294	73	79	94	rVB	106125	116108	15.56%	1.765%
3	1.555	153	160	173	rVB	103685	119264	15.99%	1.813%
4	1.741	212	218	229	rVB2	13500	18317	2.46%	0.278%
5	2.095	318	328	344	rVB2	184933	277687	37.22%	4.221%
6	2.278	378	385	394	rVB	12346	16839	2.26%	0.256%
7	2.494	443	452	465	rVB	31998	51042	6.84%	0.776%
8	2.748	521	531	551	rVB6	12647	39078	5.24%	0.594%
9	3.018	606	615	616	rBV9	7723	8794	1.18%	0.134%
10	3.182	657	666	675	rBV3	7577	14216	1.91%	0.216%
11	3.963	876	909	948	rBV2	78501	447907	60.04%	6.808%
12	4.233	984	993	1006	rVV2	5986	13592	1.82%	0.207%
13	4.336	1010	1025	1046	rVB	150380	369298	49.50%	5.613%
14	4.587	1092	1103	1111	rBV4	7605	16752	2.25%	0.255%
15	4.645	1115	1121	1133	rVB4	12364	25234	3.38%	0.384%
16	4.799	1163	1169	1188	rVB4	11312	27147	3.64%	0.413%
17	5.031	1221	1241	1267	rBV2	325492	746053	100.00%	11.340%
18	5.606	1407	1420	1448	rBV	235049	467535	62.67%	7.107%
19	5.902	1500	1512	1523	rBV6	11484	23480	3.15%	0.357%
20	6.066	1545	1563	1588	rBV	170805	378484	50.73%	5.753%
21	6.178	1588	1598	1609	rVB5	8595	17728	2.38%	0.269%
22	6.516	1693	1703	1713	rBV6	5261	10104	1.35%	0.154%
23	6.998	1842	1853	1884	rBV2	57966	121513	16.29%	1.847%
24	7.259	1922	1934	1943	rBV3	16545	30970	4.15%	0.471%
25	7.323	1943	1954	1970	rVV	234345	408922	54.81%	6.216%
26	7.397	1970	1977	1991	rVB	13352	26436	3.54%	0.402%
27	7.632	2040	2050	2072	rBV2	36404	74513	9.99%	1.133%
28	7.854	2105	2119	2129	rVB5	7904	14145	1.90%	0.215%
29	7.979	2151	2158	2170	rVB4	10963	19340	2.59%	0.294%
30	8.108	2187	2198	2233	rBV	350828	723353	96.96%	10.995%
31	8.436	2291	2300	2315	rVB2	8160	13766	1.85%	0.209%
32	8.854	2418	2430	2459	rBV	347554	597980	80.15%	9.089%
33	9.018	2472	2481	2493	rVB3	15241	24731	3.31%	0.376%
34	9.143	2511	2520	2535	rBV	13399	22651	3.04%	0.344%
35	9.551	2637	2647	2650	rBV2	15213	23471	3.15%	0.357%
36	9.934	2757	2766	2776	rBV2	14981	22360	3.00%	0.340%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026787.D
 Acq On : 15 Jul 2022 13:39
 Operator : SY/MD
 Sample : N3670-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT2-2022-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

37	10.217	2842	2854	2869	rBV	147179	240768	32.27%	3.660%
38	10.542	2944	2955	2963	rBV2	13842	20212	2.71%	0.307%
39	10.915	3063	3071	3081	rBV3	13104	20470	2.74%	0.311%
40	11.185	3142	3155	3164	rBV3	12150	19344	2.59%	0.294%
41	11.249	3164	3175	3196	rVB	302872	482975	64.74%	7.341%
42	11.622	3280	3291	3309	rBV	243846	409584	54.90%	6.226%
43	12.644	3601	3609	3619	rBV4	11775	16905	2.27%	0.257%
44	13.265	3793	3802	3810	rVB3	8452	11963	1.60%	0.182%
45	13.506	3868	3877	3888	rVB3	5224	7885	1.06%	0.120%
46	13.744	3942	3951	3963	rVB4	7760	11518	1.54%	0.175%




Sum of corrected areas: 6578915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026787.D
Acq On : 15 Jul 2022 13:39
Operator : SY/MD
Sample : N3670-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2022-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

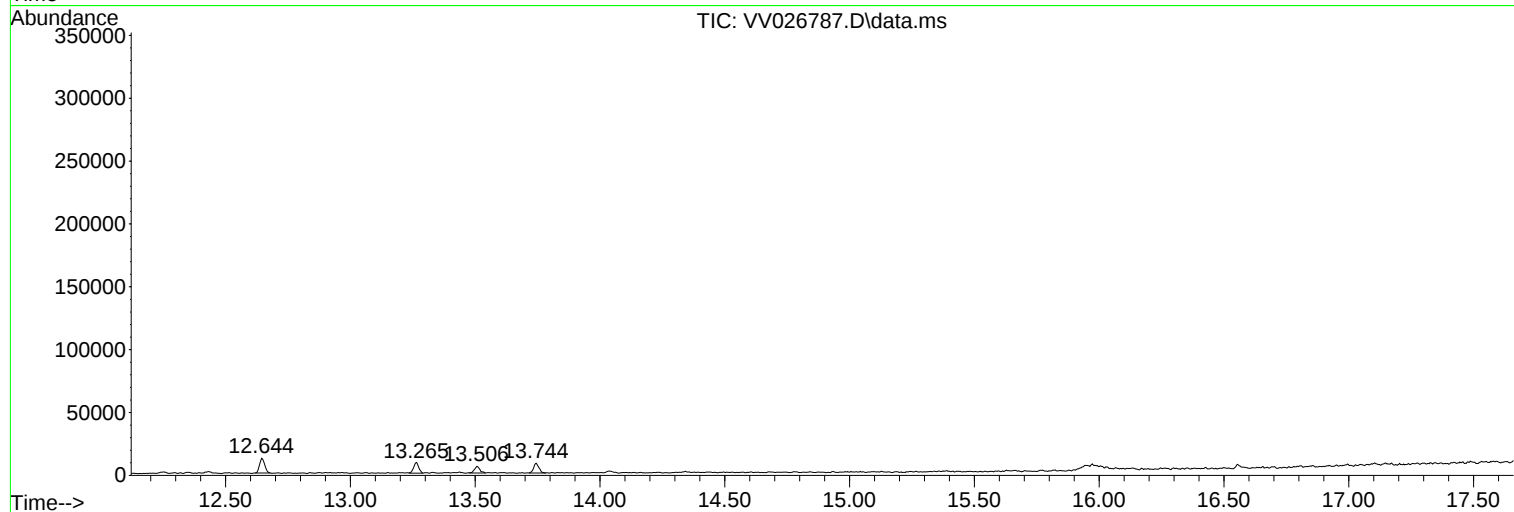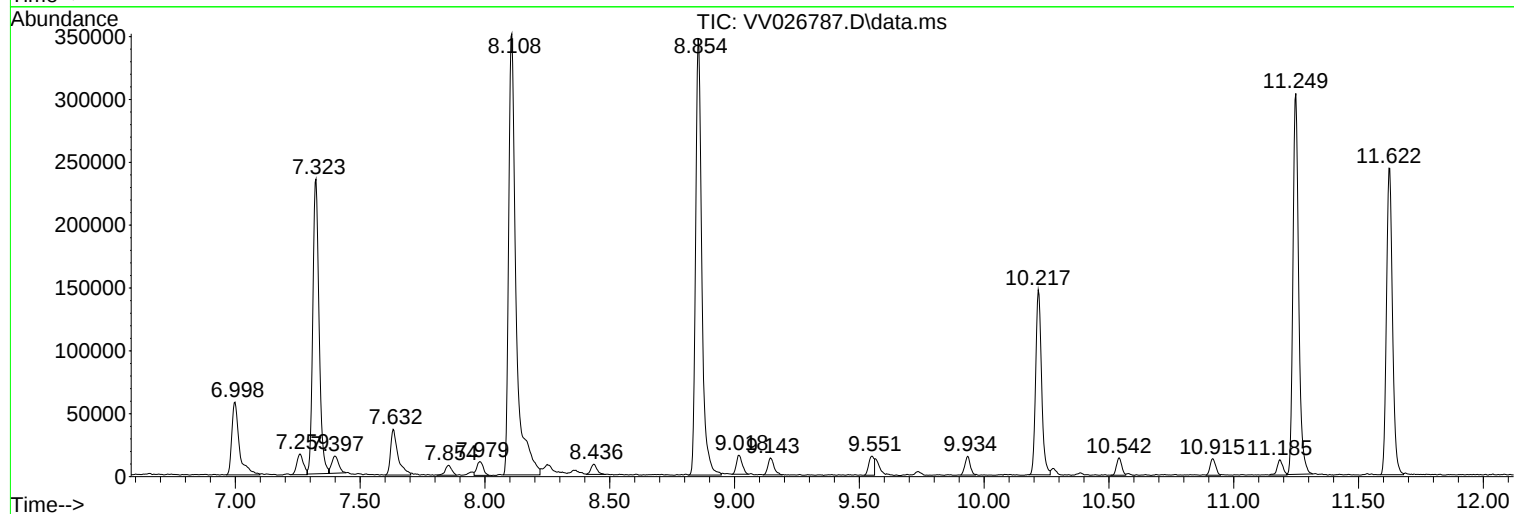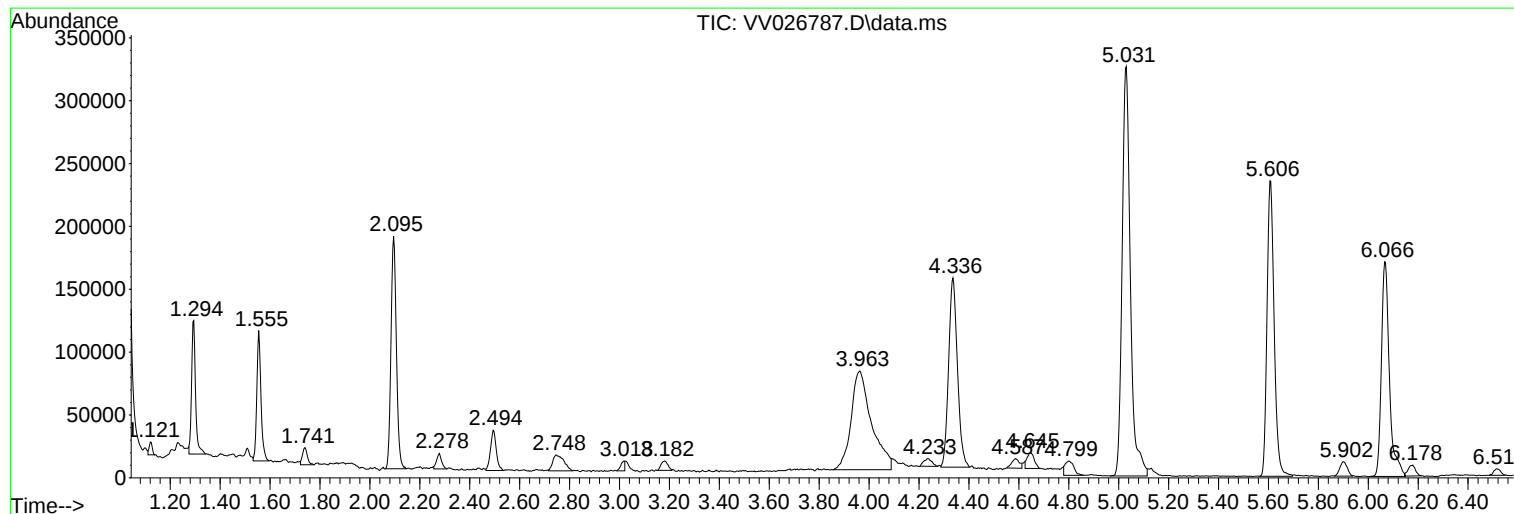

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026787.D
Acq On : 15 Jul 2022 13:39
Operator : SY/MD
Sample : N3670-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2022-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026787.D
Acq On : 15 Jul 2022 13:39
Operator : SY/MD
Sample : N3670-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2022-03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------