

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026790.D
 Acq On : 15 Jul 2022 14:54
 Operator : SY/MD
 Sample : N3710-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B38

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	94201	101763	14.09%	1.707%
2	1.564	155	163	175	rVB	98232	110957	15.37%	1.861%
3	2.101	321	330	344	rVV	163347	234592	32.49%	3.934%
4	2.201	347	361	372	rVB4	23772	45621	6.32%	0.765%
5	2.571	466	476	487	rVB3	8365	15543	2.15%	0.261%
6	3.889	876	886	919	rBV2	66002	231139	32.01%	3.876%
7	4.346	1011	1028	1060	rVB	144770	380869	52.75%	6.387%
8	5.043	1229	1245	1274	rBV2	273398	689151	95.44%	11.557%
9	5.616	1409	1423	1460	rBV	250283	529308	73.30%	8.876%
10	6.066	1550	1563	1585	rBV	179877	366871	50.81%	6.152%
11	6.985	1839	1849	1871	rBV2	59813	119351	16.53%	2.001%
12	7.313	1939	1951	1979	rBV	235731	428476	59.34%	7.185%
13	7.625	2039	2048	2064	rBV	36047	66683	9.23%	1.118%
14	8.088	2181	2192	2230	rBV	321524	722083	100.00%	12.109%
15	8.850	2418	2429	2459	rBV	403767	678481	93.96%	11.378%
16	10.214	2842	2853	2871	rBV	153645	245260	33.97%	4.113%
17	11.249	3163	3175	3194	rBV	343053	540133	74.80%	9.058%
18	11.535	3251	3264	3278	rBV6	6272	11888	1.65%	0.199%
19	11.622	3280	3291	3314	rVV	268637	430089	59.56%	7.213%
20	15.387	4454	4462	4471	rBV7	9578	14839	2.06%	0.249%




Sum of corrected areas: 5963097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026790.D
Acq On : 15 Jul 2022 14:54
Operator : SY/MD
Sample : N3710-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

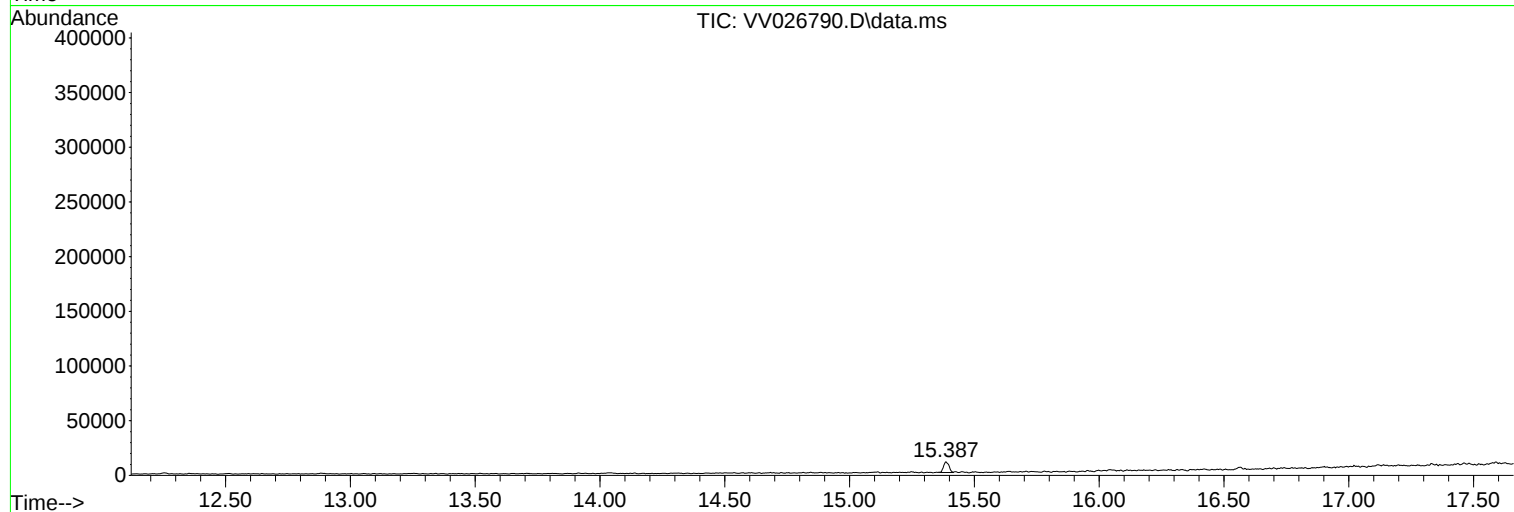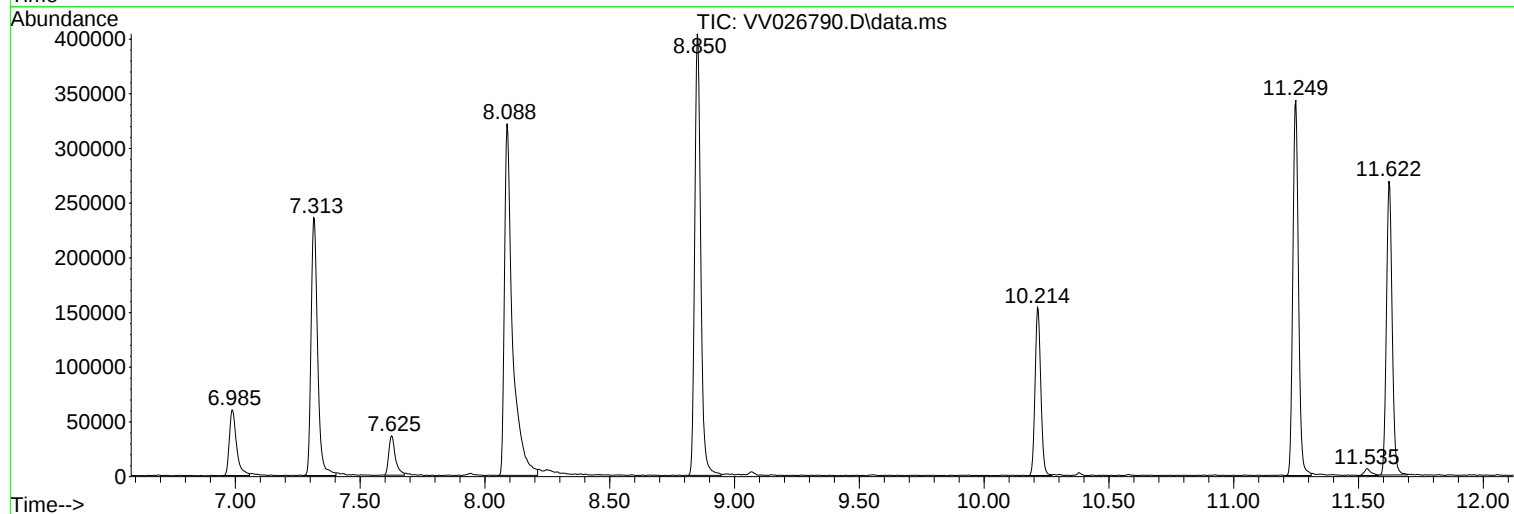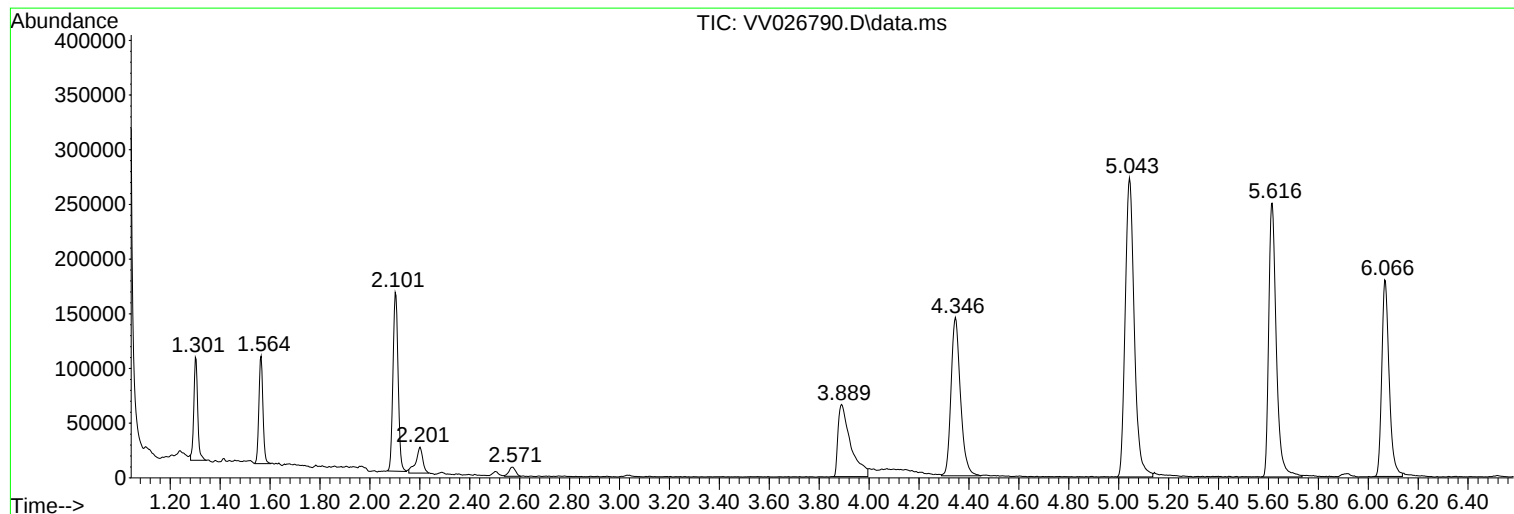

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026790.D
Acq On : 15 Jul 2022 14:54
Operator : SY/MD
Sample : N3710-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026790.D
Acq On : 15 Jul 2022 14:54
Operator : SY/MD
Sample : N3710-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
