

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026796.D
 Acq On : 15 Jul 2022 17:23
 Operator : SY/MD
 Sample : N3710-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0B44

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	74	80	94	rVB	94588	104024	13.78%	1.793%
2	1.561	155	162	175	rVB	95768	109329	14.48%	1.884%
3	2.098	319	329	343	rBV	156895	222902	29.53%	3.841%
4	3.896	877	888	922	rBV	67704	241835	32.04%	4.167%
5	4.346	1010	1028	1059	rVB	140827	382423	50.66%	6.590%
6	5.040	1227	1244	1269	rBV2	263928	668698	88.59%	11.523%
7	5.613	1410	1422	1452	rBV	232691	488489	64.71%	8.418%
8	6.066	1546	1563	1595	rBV2	175124	367638	48.70%	6.335%
9	6.986	1839	1849	1867	rBV	60194	115737	15.33%	1.994%
10	7.314	1940	1951	1971	rBV	230435	416921	55.23%	7.185%
11	7.625	2038	2048	2076	rBV	35634	70566	9.35%	1.216%
12	7.976	2150	2157	2170	rVB6	5349	9127	1.21%	0.157%
13	8.088	2182	2192	2232	rBV	340450	754862	100.00%	13.008%
14	8.850	2416	2429	2456	rBV	377014	634882	84.11%	10.941%
15	10.214	2841	2853	2875	rBV	152872	247211	32.75%	4.260%
16	11.249	3163	3175	3198	rBV	322651	508330	67.34%	8.760%
17	11.532	3252	3263	3275	rBV4	11952	23059	3.05%	0.397%
18	11.622	3280	3291	3311	rVV	269590	425953	56.43%	7.340%
19	12.345	3508	3516	3527	rBV7	6786	11053	1.46%	0.190%




Sum of corrected areas: 5803039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026796.D
Acq On : 15 Jul 2022 17:23
Operator : SY/MD
Sample : N3710-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

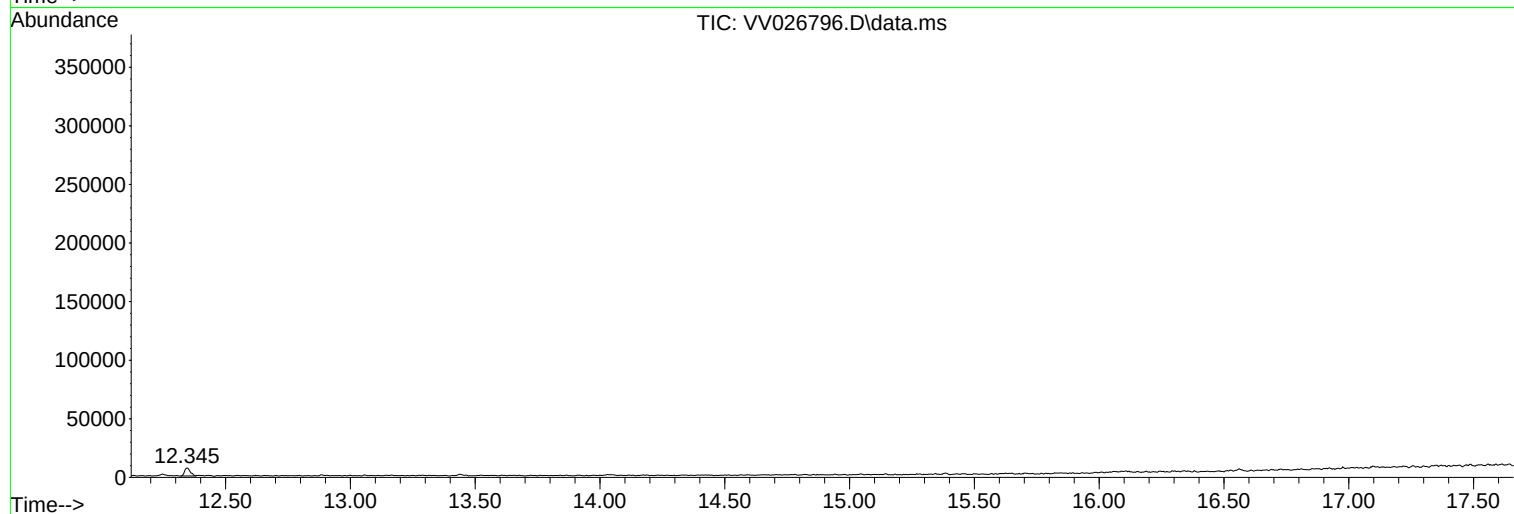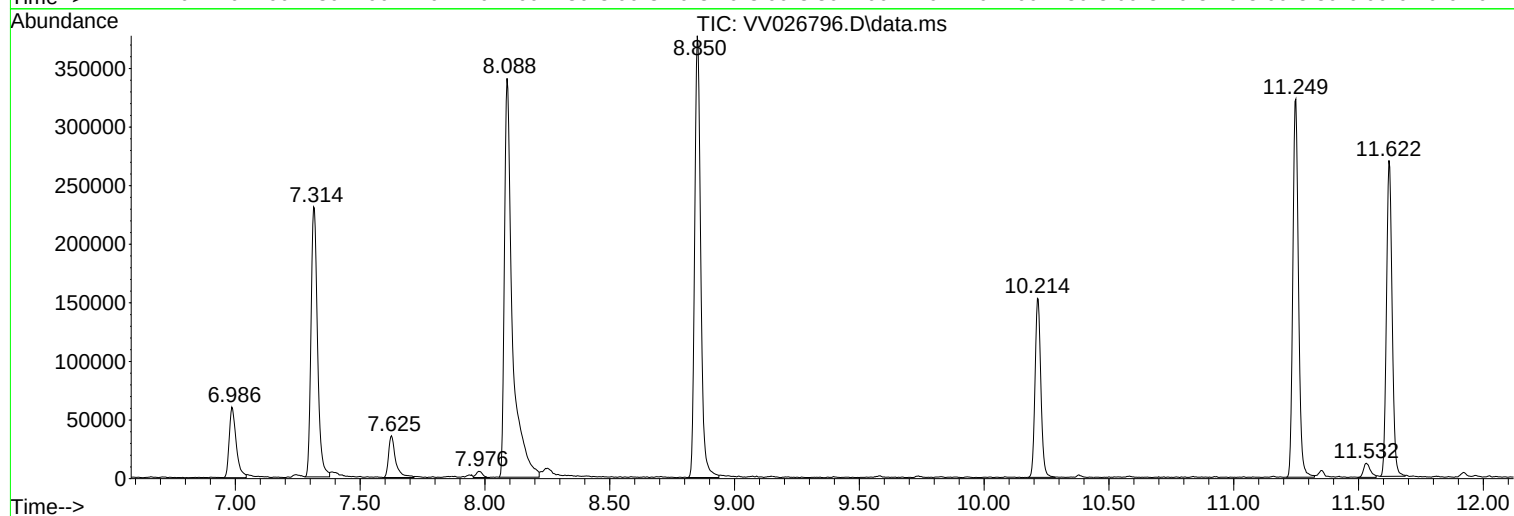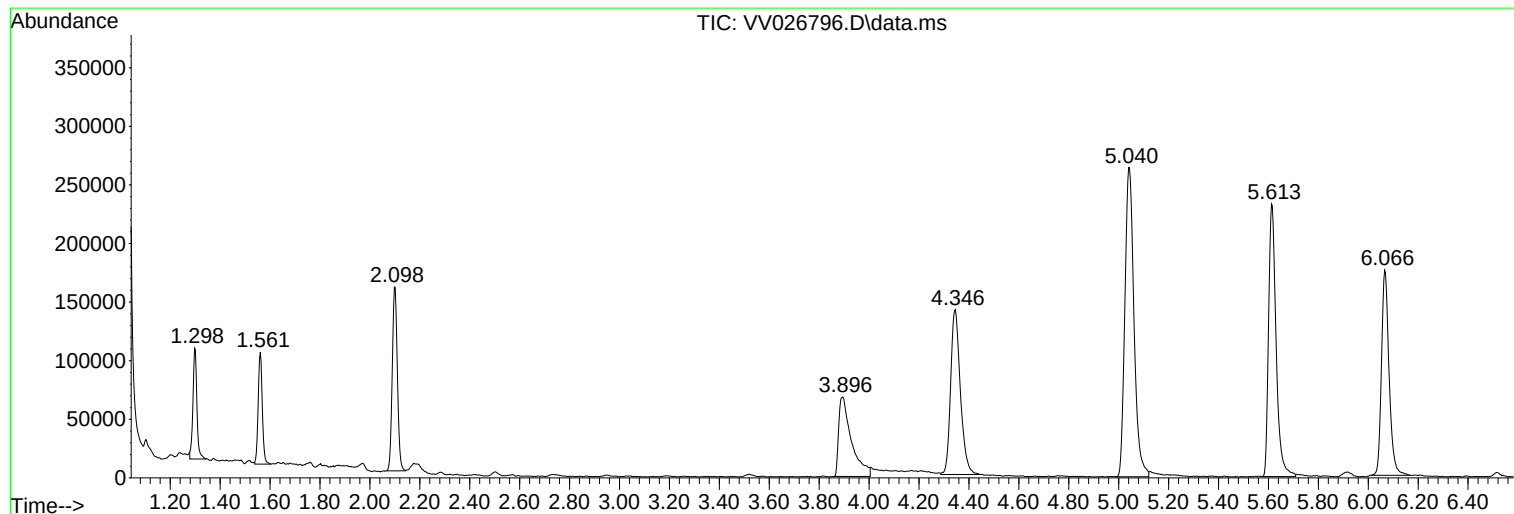

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026796.D
Acq On : 15 Jul 2022 17:23
Operator : SY/MD
Sample : N3710-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
Data File : VV026796.D
Acq On : 15 Jul 2022 17:23
Operator : SY/MD
Sample : N3710-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0B44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
