
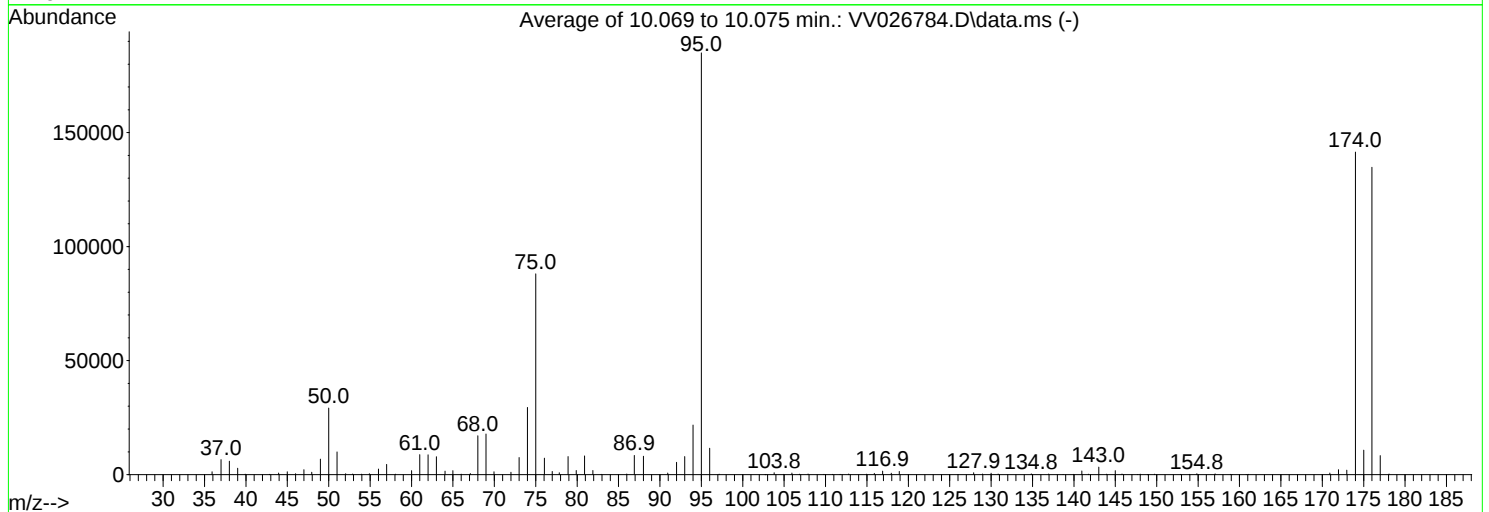


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071522\
 Data File : VV026784.D
 Acq On : 15 Jul 2022 08:43
 Operator : SY/MD
 Sample : BFB346
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB346

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jul 19 03:06:10 2022

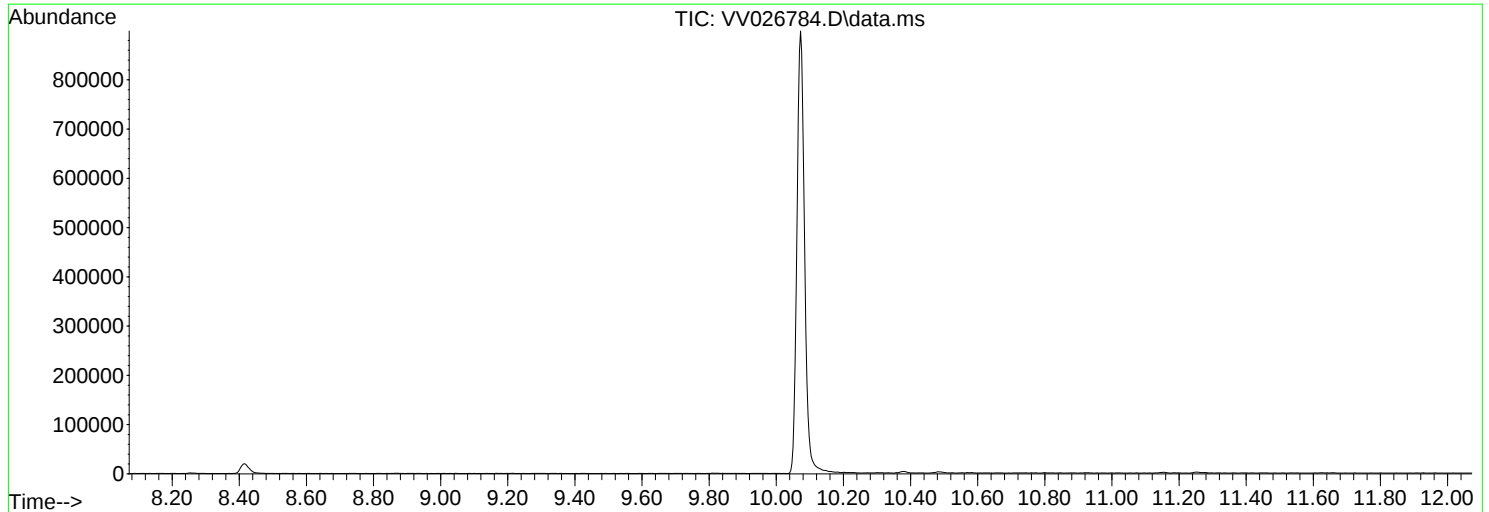

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	29181	PASS
75	95	30	80	47.6	88032	PASS
95	95	100	100	100.0	184960	PASS
96	95	5	9	6.2	11552	PASS
173	174	0.00	2	1.4	1968	PASS
174	95	50	120	76.5	141419	PASS
175	174	5	9	7.6	10709	PASS
176	174	95	105	95.3	134813	PASS
177	176	5	10	6.2	8374	PASS

m/z	Abundance
39.90	281.0
44.00	527.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346

m/z	Abundance
35.90	1249.0
37.00	6956.0
38.00	5722.0
39.00	2826.0
40.00	547.0
42.90	162.0
44.00	1196.0
45.00	1218.0
46.00	542.0
47.00	2255.0
48.00	1065.0
49.00	6583.0
50.00	29184.0
51.00	10050.0
52.00	435.0
52.90	290.0
54.00	234.0
54.90	436.0
56.00	2360.0
57.00	4529.0
58.00	250.0
60.00	1688.0
61.00	9105.0
62.00	8985.0
63.00	7780.0
64.10	1601.0
65.00	1632.0
66.00	168.0
67.10	493.0
68.00	16696.0
69.00	17488.0
70.00	1381.0
72.00	1118.0
73.00	7408.0
74.00	29096.0
75.00	86920.0
76.00	7434.0
77.00	1398.0
77.80	818.0
78.90	7920.0
79.90	1780.0
80.90	8175.0
81.90	1892.0
82.90	165.0
86.00	257.0
86.90	8100.0
88.00	8274.0
91.00	715.0
92.00	5135.0
93.00	7677.0
94.00	21504.0
95.00	183936.0
96.00	11631.0
97.20	222.0
102.70	108.0
103.80	888.0
105.00	136.0
105.90	692.0
106.80	198.0
107.90	268.0
109.80	153.0
110.90	117.0
111.80	145.0
112.80	235.0
114.90	215.0
115.90	592.0
116.90	1473.0
117.90	648.0
118.90	1372.0
126.00	135.0
127.90	800.0
129.00	324.0
130.00	623.0
130.90	288.0
134.80	308.0
136.90	313.0
138.70	104.0
139.90	134.0
140.90	1503.0
141.80	235.0
143.00	3061.0
144.00	184.0
145.00	1636.0
145.80	232.0
148.00	381.0
148.90	101.0
149.80	233.0
152.80	158.0
154.00	134.0
154.80	374.0
157.10	303.0
158.90	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346

160.80	172.0
170.90	781.0
172.00	2116.0
172.90	1886.0
174.00	137408.0
175.00	10361.0
176.00	129432.0
177.00	8247.0
178.10	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346

m/z	Abundance
35.90	1319.0
37.00	6821.0
38.00	6122.0
39.00	2876.0
39.90	498.0
42.90	162.0
44.00	1188.0
45.00	1333.0
46.00	475.0
47.00	2285.0
48.00	1081.0
49.00	7033.0
50.00	30032.0
51.00	10409.0
52.10	436.0
52.90	305.0
54.00	242.0
54.90	461.0
56.00	2491.0
57.00	4601.0
58.00	241.0
60.00	1780.0
61.00	9006.0
62.00	9085.0
63.00	8097.0
64.00	1560.0
65.00	1794.0
66.00	208.0
67.10	519.0
68.00	17760.0
69.00	18472.0
69.90	1294.0
72.00	1061.0
73.00	7715.0
74.00	30528.0
75.00	90680.0
76.10	7369.0
77.00	1558.0
77.90	860.0
78.90	8081.0
79.90	1934.0
80.90	8437.0
81.90	1912.0
82.90	175.0
86.00	322.0
86.90	8672.0
88.00	8242.0
90.90	741.0
92.00	5668.0
93.00	8150.0
94.00	22584.0
95.00	191488.0
96.00	11895.0
97.20	170.0
103.80	890.0
104.90	138.0
106.00	710.0
106.80	204.0
107.90	275.0
109.80	117.0
110.80	177.0
111.80	112.0
112.80	257.0
115.00	194.0
115.90	597.0
116.90	1624.0
118.00	635.0
118.90	1505.0
126.00	117.0
127.90	883.0
128.90	335.0
130.00	640.0
130.80	260.0
134.90	331.0
137.00	313.0
138.70	106.0
140.00	144.0
141.00	1646.0
141.80	216.0
143.00	3400.0
144.00	199.0
145.00	1878.0
145.80	273.0
148.00	350.0
149.80	219.0
152.90	136.0
153.90	131.0
154.90	478.0
157.00	357.0
158.90	221.0
161.00	172.0
170.90	748.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346

172.00	2270.0
172.90	2076.0
174.00	145984.0
175.00	11144.0
176.00	139520.0
177.00	8567.0
178.00	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346

m/z	Abundance
35.90	1243.0
37.00	6003.0
38.00	5945.0
39.00	2710.0
39.90	519.0
42.80	122.0
43.90	1214.0
45.00	1261.0
46.00	321.0
47.00	1969.0
47.90	1069.0
49.00	6812.0
50.00	28328.0
51.00	9538.0
52.10	384.0
52.90	290.0
53.90	241.0
54.90	463.0
56.00	2422.0
57.00	4311.0
58.10	209.0
60.00	1719.0
61.00	8134.0
62.00	8113.0
63.00	7673.0
64.00	1412.0
65.00	1812.0
66.00	246.0
67.10	447.0
68.00	16696.0
69.00	17600.0
69.90	1129.0
72.00	976.0
73.00	7390.0
74.00	28816.0
75.00	86496.0
76.10	6860.0
77.00	1355.0
77.90	784.0
78.90	7817.0
79.90	1872.0
80.90	7966.0
81.90	1708.0
82.90	180.0
86.00	293.0
86.90	8572.0
88.00	7694.0
90.90	717.0
92.00	5333.0
93.00	7940.0
94.00	21216.0
95.00	179456.0
96.00	11129.0
97.00	225.0
103.80	804.0
104.90	169.0
106.00	653.0
106.90	211.0
107.90	259.0
109.80	115.0
110.80	201.0
111.70	119.0
112.80	251.0
115.00	202.0
115.90	578.0
116.90	1599.0
117.90	597.0
118.90	1414.0
127.90	799.0
128.90	298.0
130.00	632.0
130.80	221.0
134.90	323.0
136.90	330.0
140.00	155.0
141.00	1619.0
141.70	216.0
143.00	3381.0
143.90	184.0
145.00	1747.0
145.80	264.0
147.70	297.0
149.70	174.0
153.00	145.0
153.90	127.0
154.90	477.0
157.00	350.0
159.10	162.0
161.10	186.0
170.90	653.0
171.90	2201.0
173.00	1941.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346

174.00	140864.0
175.00	10622.0
176.00	135488.0
177.00	8307.0
178.00	308.0

Instrument :
MSVOA_V
ClientSampleId :
BFB346