
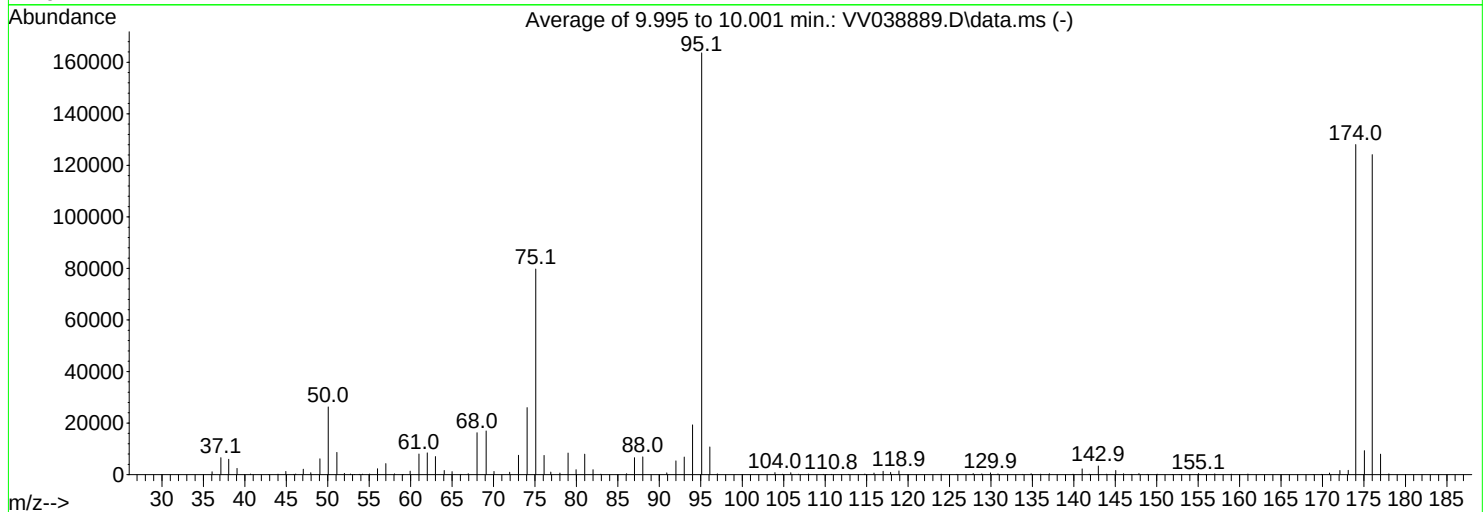


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV071525\
Data File : VV038889.D
Acq On : 15 Jul 2025 07:55
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V071125W.M
Title : SW846 8260
Last Update : Mon Jul 14 09:44:44 2025

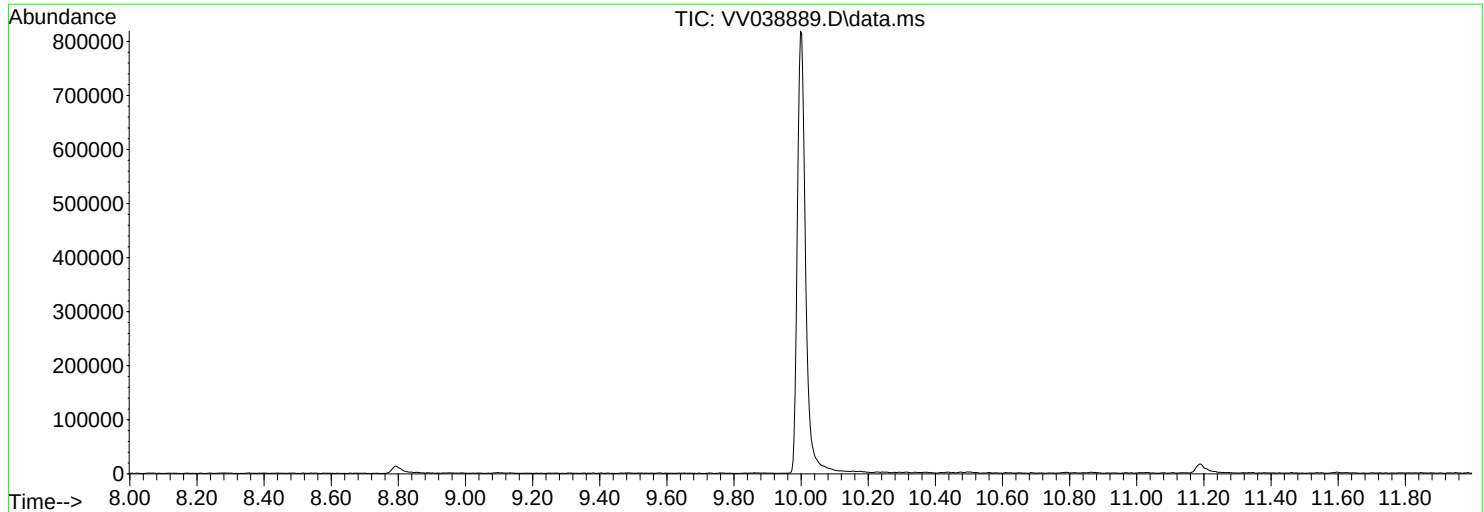

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	26280	PASS
75	95	30	60	48.8	79784	PASS
95	95	100	100	100.0	163648	PASS
96	95	5	9	6.6	10722	PASS
173	174	0.00	2	1.3	1658	PASS
174	95	50	100	78.3	128088	PASS
175	174	5	9	7.3	9300	PASS
176	174	95	101	96.9	124139	PASS
177	176	5	9	6.4	7968	PASS