
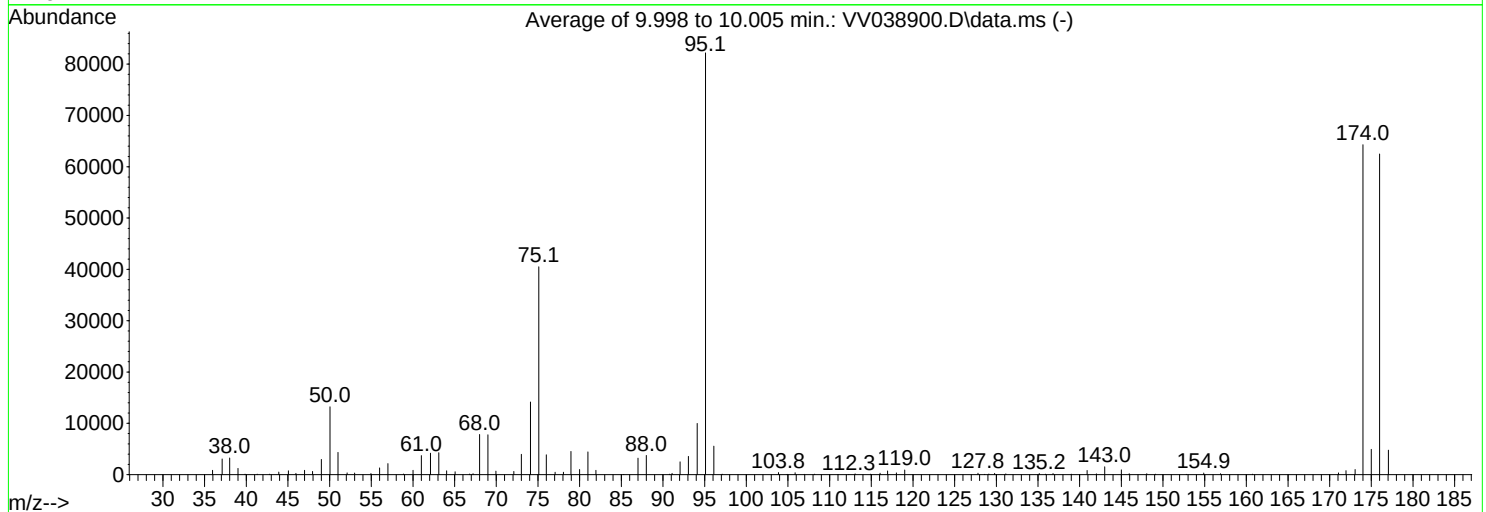


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV071625\
Data File : VV038900.D
Acq On : 16 Jul 2025 09:13
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V071125W.M
Title : SW846 8260
Last Update : Mon Jul 14 09:44:44 2025

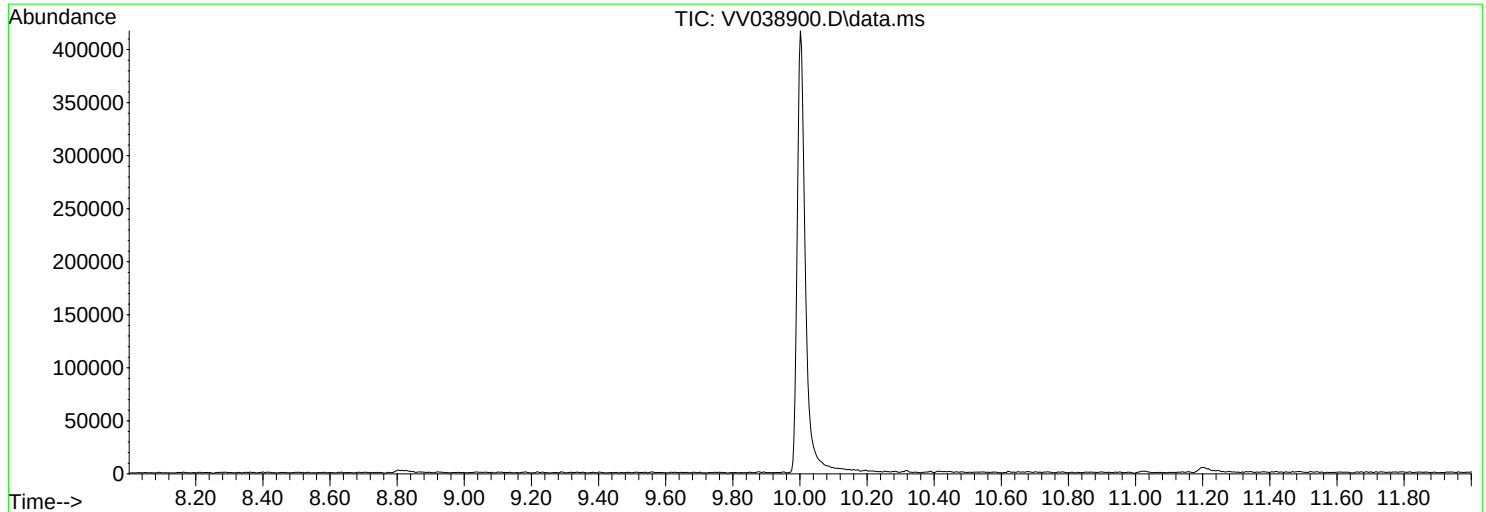

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	13231	PASS
75	95	30	60	49.3	40496	PASS
95	95	100	100	100.0	82195	PASS
96	95	5	9	6.8	5566	PASS
173	174	0.00	2	1.6	1004	PASS
174	95	50	100	78.2	64285	PASS
175	174	5	9	7.7	4932	PASS
176	174	95	101	97.2	62477	PASS
177	176	5	9	7.6	4773	PASS