


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071718\
 Data File : VV006612.D
 Acq On : 17 Jul 2018 11:00
 Operator : SY/MD
 Sample : BFB66
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB66

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jul 17 15:32:48 2018

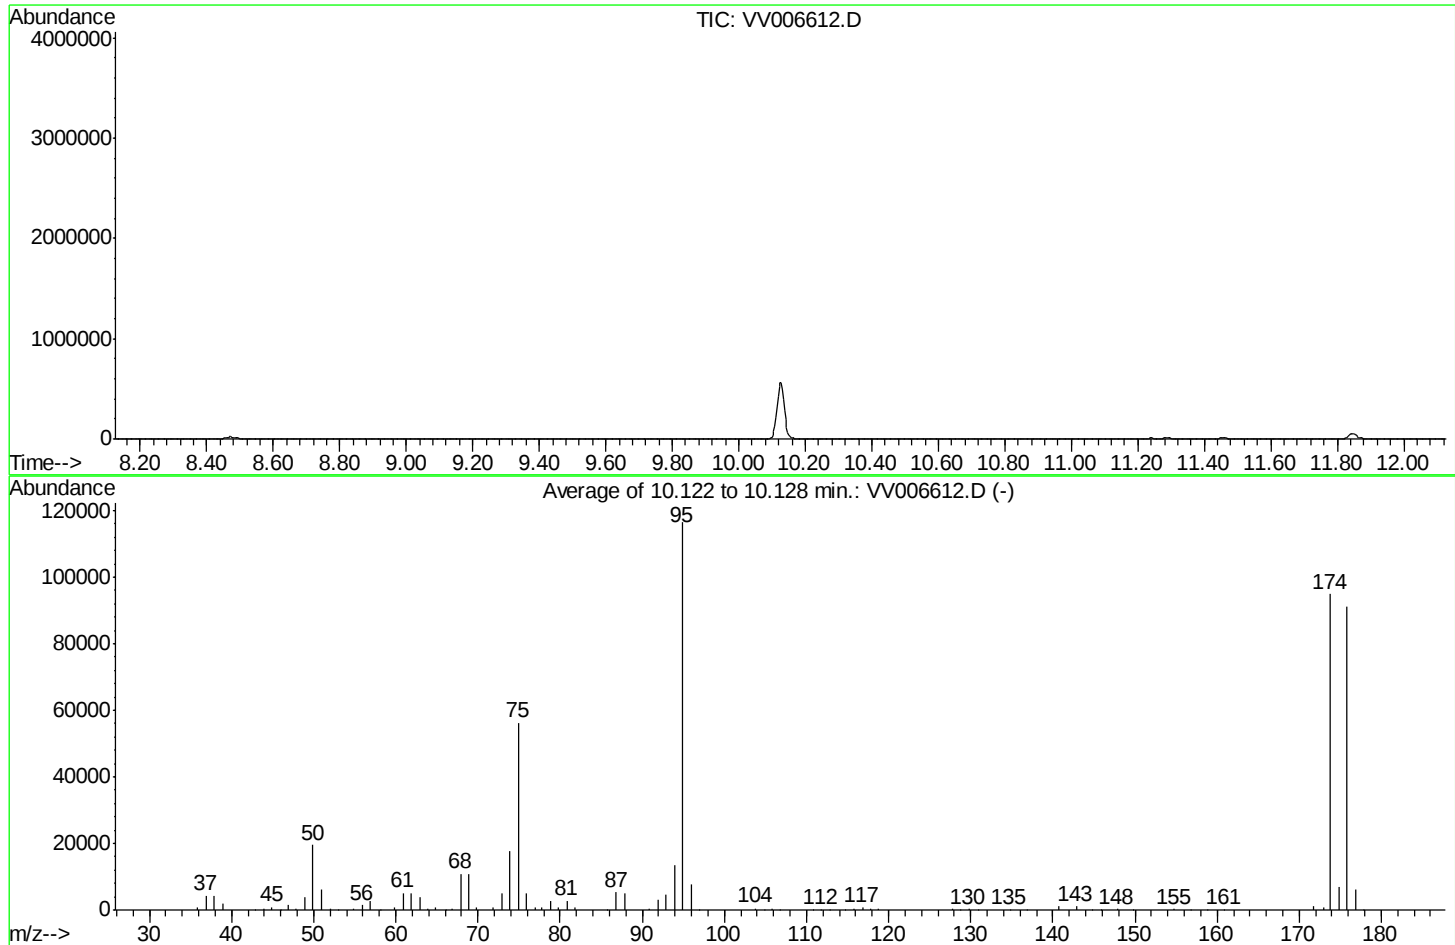

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	19453	PASS
75	95	30	80	48.2	56149	PASS
95	95	100	100	100.0	116464	PASS
96	95	5	9	6.6	7665	PASS
173	174	0.00	2	1.0	958	PASS
174	95	50	120	81.5	94866	PASS
175	174	5	9	7.3	6918	PASS
176	174	95	101	96.1	91200	PASS
177	176	5	9	6.7	6134	PASS

Scan 2858 (10.080 min): VV006612.D
BFB66

m/z	Abundance
39.90	223.0
40.90	102.0
43.00	104.0
43.90	702.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	697.0
36.90	4242.0
37.90	4197.0
38.90	1893.0
39.90	217.0
42.80	127.0
43.90	1169.0
44.90	922.0
46.00	145.0
46.90	1542.0
47.80	488.0
48.90	3784.0
49.90	18688.0
50.90	6103.0
52.00	258.0
52.90	146.0
54.90	266.0
55.90	1276.0
56.90	2557.0
58.10	140.0
59.90	864.0
60.90	4933.0
61.90	4796.0
62.90	3640.0
63.90	466.0
64.80	693.0
66.90	266.0
67.90	10745.0
68.90	10227.0
69.80	806.0
71.80	592.0
72.90	4773.0
73.90	17232.0
74.90	53928.0
75.90	4779.0
77.00	757.0
77.80	655.0
78.90	2534.0
79.80	777.0
80.80	2608.0
81.80	591.0
85.80	191.0
86.90	4975.0
87.90	4720.0
90.80	386.0
91.90	2948.0
92.90	4348.0
93.90	12928.0
94.90	111128.0
95.90	7391.0
96.90	222.0
103.80	398.0
104.80	168.0
105.80	379.0
112.80	109.0
114.70	110.0
115.80	340.0
116.80	586.0
117.80	391.0
118.80	502.0
127.80	341.0
128.70	199.0
129.70	356.0
130.90	147.0
134.80	178.0
136.80	144.0
140.80	955.0
142.80	975.0
144.80	194.0
145.90	129.0
147.90	310.0
154.80	284.0
156.80	147.0
158.80	118.0
171.80	937.0
173.00	889.0
173.80	87552.0
174.90	6402.0
175.80	84520.0
176.90	5718.0
177.80	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	746.0
36.90	4490.0
37.90	4440.0
38.90	1991.0
39.80	220.0
42.80	125.0
43.90	1155.0
44.90	977.0
45.90	165.0
46.90	1518.0
47.90	567.0
48.90	4012.0
49.90	20176.0
50.90	6554.0
52.00	267.0
52.90	164.0
54.80	274.0
55.90	1442.0
56.90	2669.0
58.10	170.0
59.90	971.0
60.90	5283.0
61.90	5105.0
62.90	3884.0
63.80	507.0
64.80	754.0
66.00	112.0
66.80	285.0
67.90	11293.0
68.90	11176.0
69.90	883.0
71.80	662.0
72.90	5328.0
73.90	18232.0
74.90	57960.0
75.90	5103.0
76.90	811.0
77.80	654.0
78.90	2694.0
79.90	868.0
80.80	2862.0
81.80	649.0
85.70	177.0
86.80	5421.0
87.90	5271.0
90.80	406.0
91.90	3138.0
92.90	4753.0
93.90	13959.0
94.90	120448.0
95.90	7912.0
96.90	190.0
103.80	432.0
104.80	159.0
105.80	424.0
106.80	128.0
110.70	112.0
111.80	118.0
114.70	102.0
115.80	394.0
116.80	669.0
117.80	408.0
118.80	552.0
127.80	374.0
128.70	205.0
129.80	397.0
130.90	178.0
134.80	191.0
136.80	175.0
140.80	1020.0
142.90	1126.0
144.70	221.0
145.80	150.0
147.90	319.0
149.70	102.0
154.80	300.0
156.80	157.0
158.70	147.0
160.90	121.0
171.80	1036.0
172.90	979.0
173.80	98168.0
174.90	7185.0
175.80	94352.0
176.90	6381.0
177.80	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	791.0
36.90	4307.0
37.90	4186.0
38.90	1924.0
39.80	227.0
43.00	124.0
43.80	1111.0
44.90	901.0
45.90	184.0
46.90	1364.0
47.80	612.0
48.90	3908.0
49.90	19496.0
50.90	6330.0
52.00	257.0
52.90	156.0
54.80	263.0
55.90	1426.0
56.90	2594.0
58.10	152.0
59.90	960.0
60.90	4951.0
61.90	4952.0
62.90	3822.0
63.80	488.0
64.80	739.0
66.00	119.0
66.80	293.0
67.90	10576.0
68.90	11126.0
69.90	856.0
71.90	658.0
72.90	5201.0
73.90	17600.0
74.90	56560.0
75.90	4894.0
76.90	779.0
77.80	538.0
78.90	2652.0
79.90	847.0
80.80	2802.0
81.80	646.0
85.70	183.0
86.80	5358.0
87.90	5276.0
90.80	368.0
91.90	2994.0
92.90	4608.0
93.90	13488.0
94.90	117816.0
96.00	7693.0
96.90	178.0
103.80	426.0
104.80	140.0
105.80	429.0
106.80	142.0
110.80	113.0
111.80	141.0
115.80	396.0
116.80	685.0
117.90	408.0
118.80	546.0
127.80	345.0
128.80	211.0
129.80	404.0
130.90	187.0
134.80	190.0
136.80	196.0
140.80	986.0
142.90	1092.0
144.70	203.0
145.80	161.0
147.80	279.0
149.80	103.0
154.80	271.0
156.80	150.0
158.70	161.0
160.90	141.0
171.80	1035.0
172.90	1008.0
173.80	98880.0
174.90	7169.0
175.90	94728.0
176.90	6303.0
177.80	174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66