


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071719\
Data File : VV011900.D
Acq On : 17 Jul 2019 09:39
Operator : SY/MD
Sample : BFB34
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Title : VOC Analysis
Last Update : Thu Jul 18 06:37:55 2019

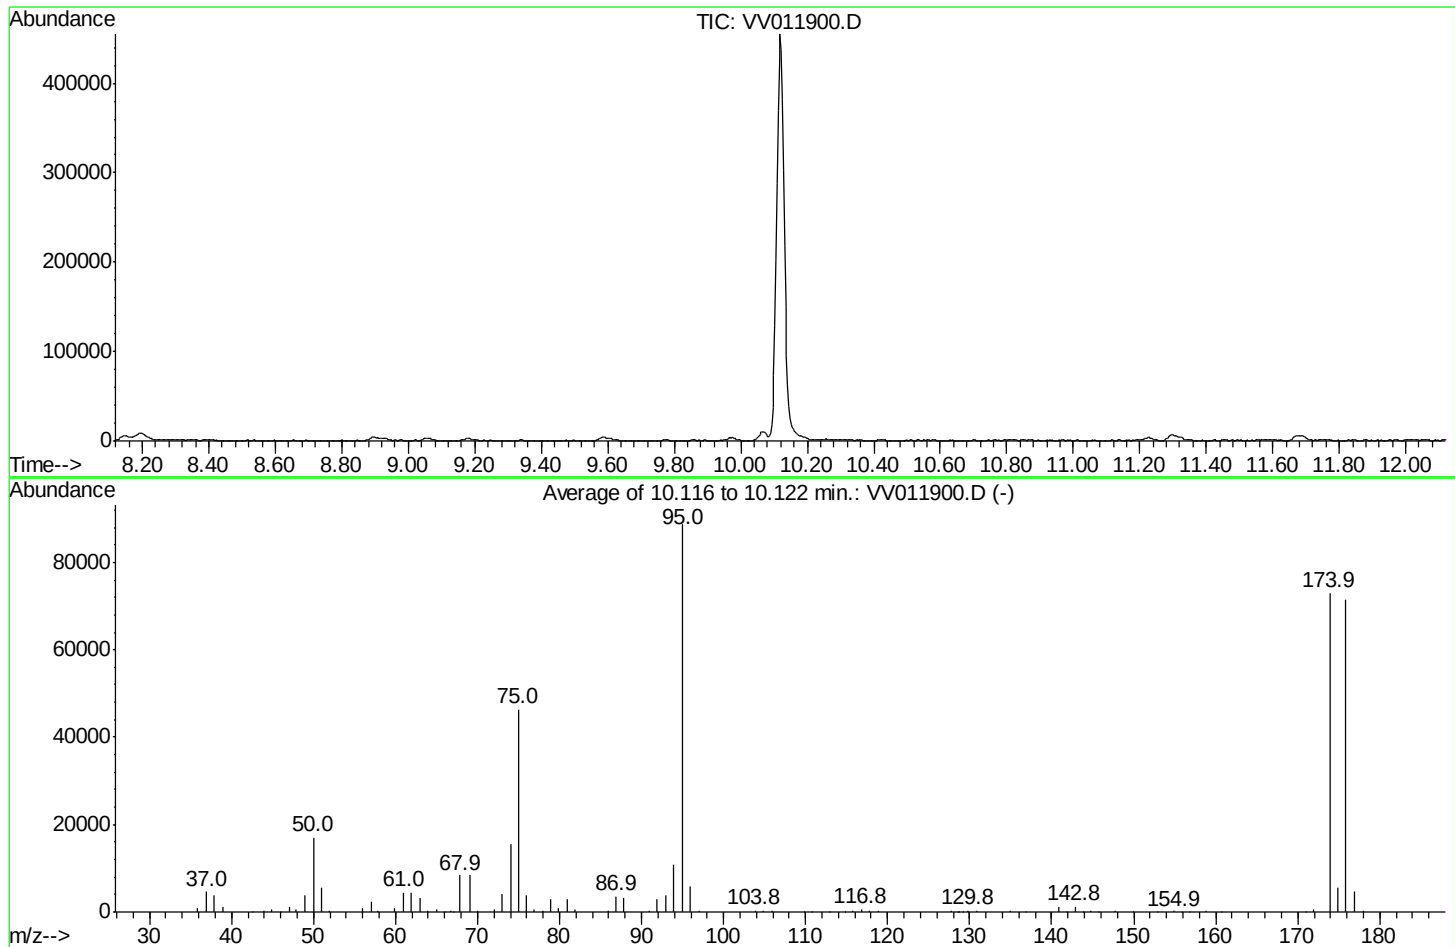

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	17018	PASS
75	95	30	80	52.3	46368	PASS
95	95	100	100	100.0	88701	PASS
96	95	5	9	6.7	5905	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.4	73077	PASS
175	174	5	9	7.7	5632	PASS
176	174	95	101	97.7	71360	PASS
177	176	5	9	6.7	4812	PASS

Scan 2795 (10.077 min): VV011900.D
BFB34

m/z	Abundance
38.10	108.0
38.90	486.0
39.90	504.0
40.90	496.0
41.90	995.0
42.90	255.0
44.00	309.0
52.80	148.0
53.80	165.0
54.90	1380.0
56.10	207.0
67.80	161.0
69.00	464.0
69.90	472.0
83.20	155.0
95.90	120.0
97.90	667.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
35.90	759.0
37.00	4576.0
37.90	3887.0
39.00	1758.0
39.90	368.0
40.90	136.0
42.00	130.0
44.00	665.0
45.00	659.0
45.90	112.0
46.90	1068.0
47.80	665.0
48.90	3549.0
50.00	16800.0
51.00	5450.0
52.00	260.0
54.90	376.0
56.00	1185.0
57.00	2443.0
57.90	160.0
59.90	874.0
61.00	4480.0
61.90	4352.0
63.00	3272.0
64.00	430.0
65.00	524.0
66.00	108.0
66.80	274.0
67.90	8613.0
69.00	8716.0
70.00	822.0
72.00	523.0
72.90	3905.0
74.00	15344.0
75.00	45544.0
76.00	3932.0
76.80	535.0
78.00	383.0
78.90	2925.0
79.90	778.0
80.90	2951.0
81.90	606.0
86.00	178.0
86.90	3533.0
87.90	3254.0
90.90	321.0
91.90	2878.0
93.00	3671.0
93.90	10825.0
95.00	87224.0
96.00	5917.0
97.00	182.0
103.80	432.0
104.80	151.0
105.80	382.0
110.80	149.0
114.90	120.0
115.70	309.0
116.80	667.0
117.80	358.0
118.90	411.0
127.80	331.0
128.50	120.0
129.10	119.0
129.80	406.0
130.80	201.0
134.90	190.0
136.80	159.0
140.80	1116.0
142.90	1185.0
144.80	201.0
145.70	124.0
147.70	265.0
149.90	102.0
152.90	139.0
154.90	226.0
156.70	146.0
158.70	194.0
160.70	147.0
171.00	119.0
171.80	697.0
173.90	69208.0
174.90	5723.0
175.90	68456.0
176.90	4509.0
178.00	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
35.90	767.0
37.00	4836.0
37.90	4093.0
39.00	1756.0
39.80	343.0
40.90	136.0
42.00	115.0
43.90	646.0
45.00	735.0
45.90	126.0
47.00	1078.0
47.90	686.0
48.90	4032.0
50.00	17496.0
50.90	5635.0
52.00	272.0
52.60	113.0
54.90	440.0
56.00	1237.0
57.00	2548.0
57.90	160.0
59.90	815.0
61.00	4526.0
61.90	4627.0
63.00	3225.0
64.00	448.0
65.00	482.0
66.80	264.0
68.00	8769.0
69.00	9032.0
70.00	890.0
72.00	559.0
73.00	4087.0
74.00	16277.0
75.00	47840.0
76.00	3998.0
76.80	599.0
78.00	320.0
78.90	3035.0
79.90	803.0
80.90	3103.0
81.90	584.0
86.00	175.0
86.90	3704.0
87.90	3199.0
91.00	377.0
91.90	3067.0
93.00	3867.0
94.00	11138.0
95.00	91680.0
96.00	6209.0
97.00	193.0
103.90	461.0
104.90	165.0
105.90	376.0
109.80	103.0
110.80	137.0
113.00	139.0
114.90	111.0
115.80	292.0
116.80	727.0
117.80	377.0
118.90	470.0
127.80	334.0
128.50	120.0
129.80	403.0
130.80	198.0
134.90	193.0
136.90	161.0
140.80	1095.0
141.80	122.0
142.80	1231.0
143.80	111.0
144.80	205.0
145.60	135.0
147.70	256.0
149.80	108.0
152.90	128.0
155.00	274.0
156.70	135.0
158.70	210.0
160.70	156.0
171.10	115.0
171.90	743.0
173.90	75456.0
174.90	5801.0
175.90	73848.0
176.90	4970.0
178.00	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
35.90	752.0
37.00	4469.0
37.90	3863.0
39.00	1625.0
39.80	307.0
41.00	120.0
42.00	124.0
42.50	113.0
43.90	649.0
44.90	756.0
46.00	121.0
47.10	1137.0
47.90	587.0
48.90	4099.0
50.00	16760.0
50.90	5478.0
51.90	257.0
52.70	129.0
54.90	440.0
56.00	1217.0
57.00	2432.0
57.90	155.0
59.90	694.0
61.00	4418.0
61.90	4284.0
63.00	3021.0
63.90	423.0
65.00	415.0
67.00	237.0
68.00	8334.0
69.00	8747.0
70.00	803.0
72.00	489.0
73.00	4083.0
74.00	15371.0
75.00	45720.0
76.00	3686.0
76.90	675.0
77.80	314.0
78.90	2792.0
79.80	738.0
80.90	2797.0
81.90	549.0
85.90	151.0
86.90	3582.0
87.80	2952.0
90.90	409.0
91.90	2918.0
93.00	3739.0
94.00	10435.0
95.00	87200.0
96.00	5951.0
97.00	176.0
103.80	436.0
104.90	165.0
105.90	351.0
110.80	132.0
113.00	140.0
114.70	104.0
115.90	321.0
116.80	673.0
117.80	340.0
118.90	467.0
127.80	319.0
128.70	141.0
129.80	383.0
130.80	182.0
134.90	173.0
136.70	141.0
140.80	987.0
141.80	125.0
142.80	1151.0
143.80	147.0
144.80	167.0
145.60	124.0
147.80	213.0
149.80	109.0
155.00	285.0
155.80	125.0
156.80	140.0
158.80	174.0
160.80	155.0
172.00	747.0
173.90	74568.0
174.90	5373.0
175.90	71776.0
176.90	4959.0
178.00	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34