
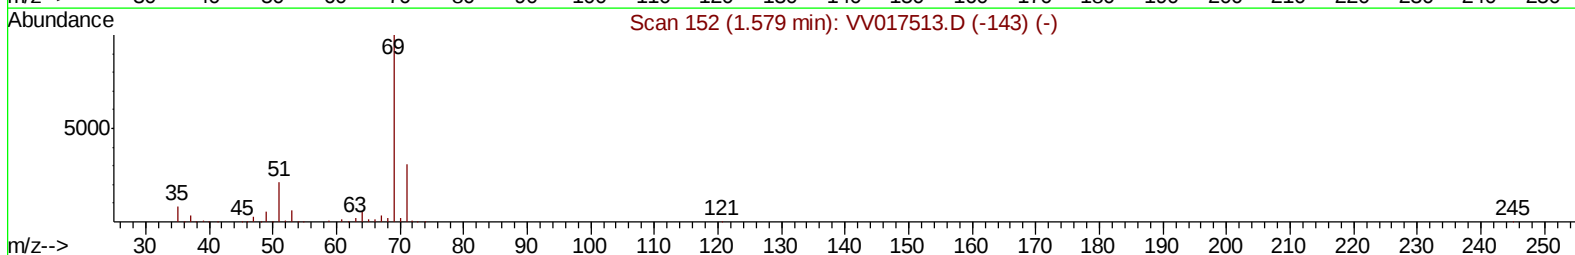
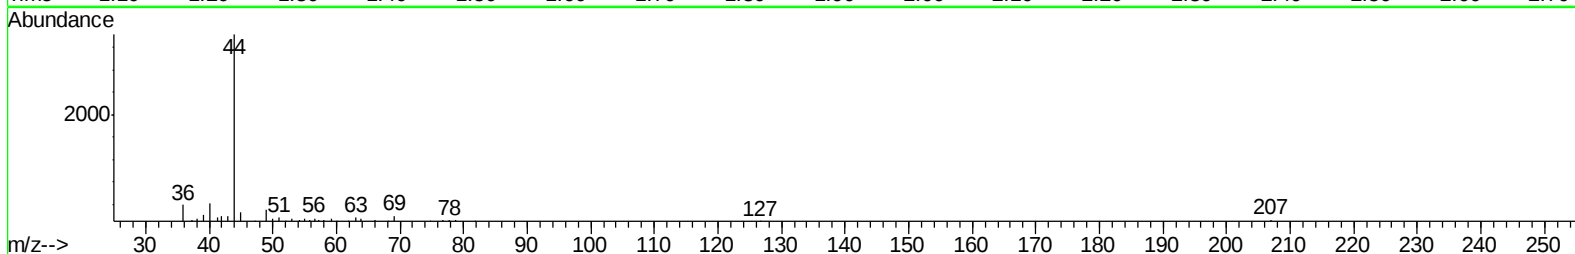


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV017533.D
 Acq On : 17 Jul 2020 19:00
 Operator : SY/MD
 Sample : L3336-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Quant Time: Jul 18 05:11:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 18 05:06:25 2020
 Response via : Initial Calibration

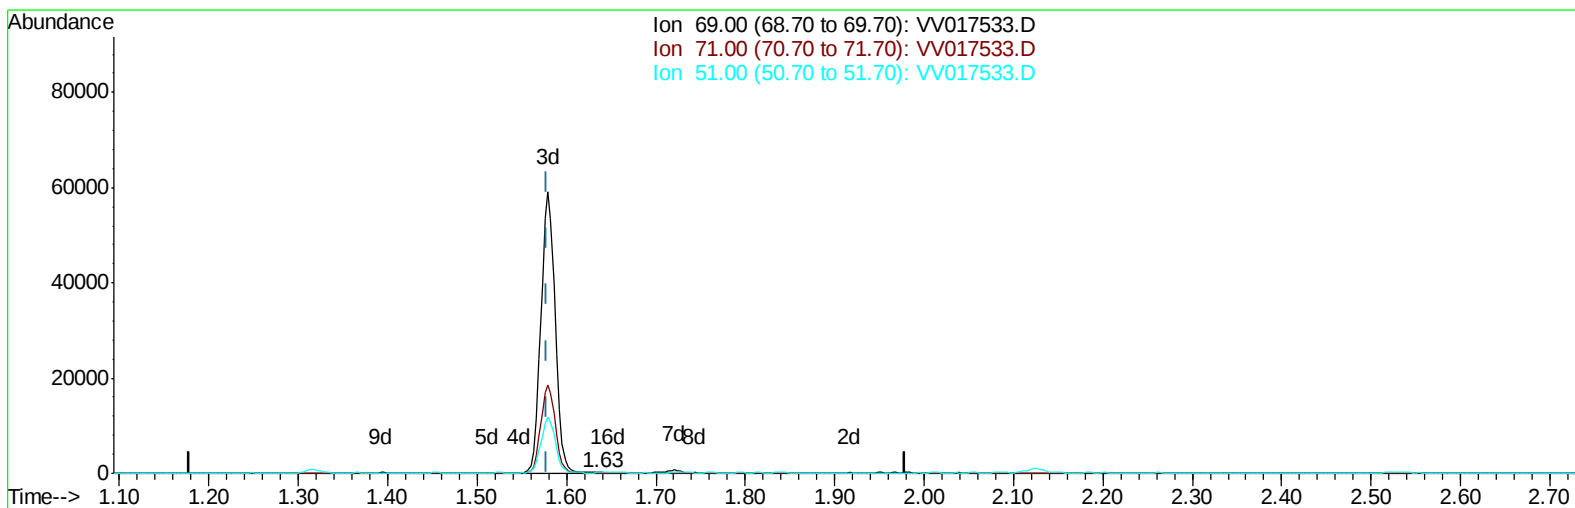

TIC: VV017533.D

(7) Chloroethane-d5 (S)

1.634min (+0.055) 0.15ug/L

response 185

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	23.24
51.00	31.70	34.59
0.00	0.00	0.00